


0831-3
A1D

8.85
8.84
8.39
8.28
8.27
8.04
8.03
7.79
7.66
7.53
7.51

Parameter	Value
1 Origin	Bruker BioSpin GmbH
2 Owner	root
3 Solvent	DMSO
4 Temperature	298.1
5 Pulse Sequence	zg30
6 Receiver Gain	137
7 Relaxation Delay	1.0000
8 Pulse Width	8.0000
9 Acquisition Time	3.2768
10 Acquisition Date	2017-09-01T08:41:01
11 Modification Date	2017-09-01T08:41:02
12 Spectrometer Frequency	500.13
13 Spectral Width	10000.0
14 Lowest Frequency	-1911.7
15 Nucleus	1H
16 Acquired Size	32768
17 Spectral Size	65536

4.30
3.74
2.51
2.51
2.51
2.49
2.38

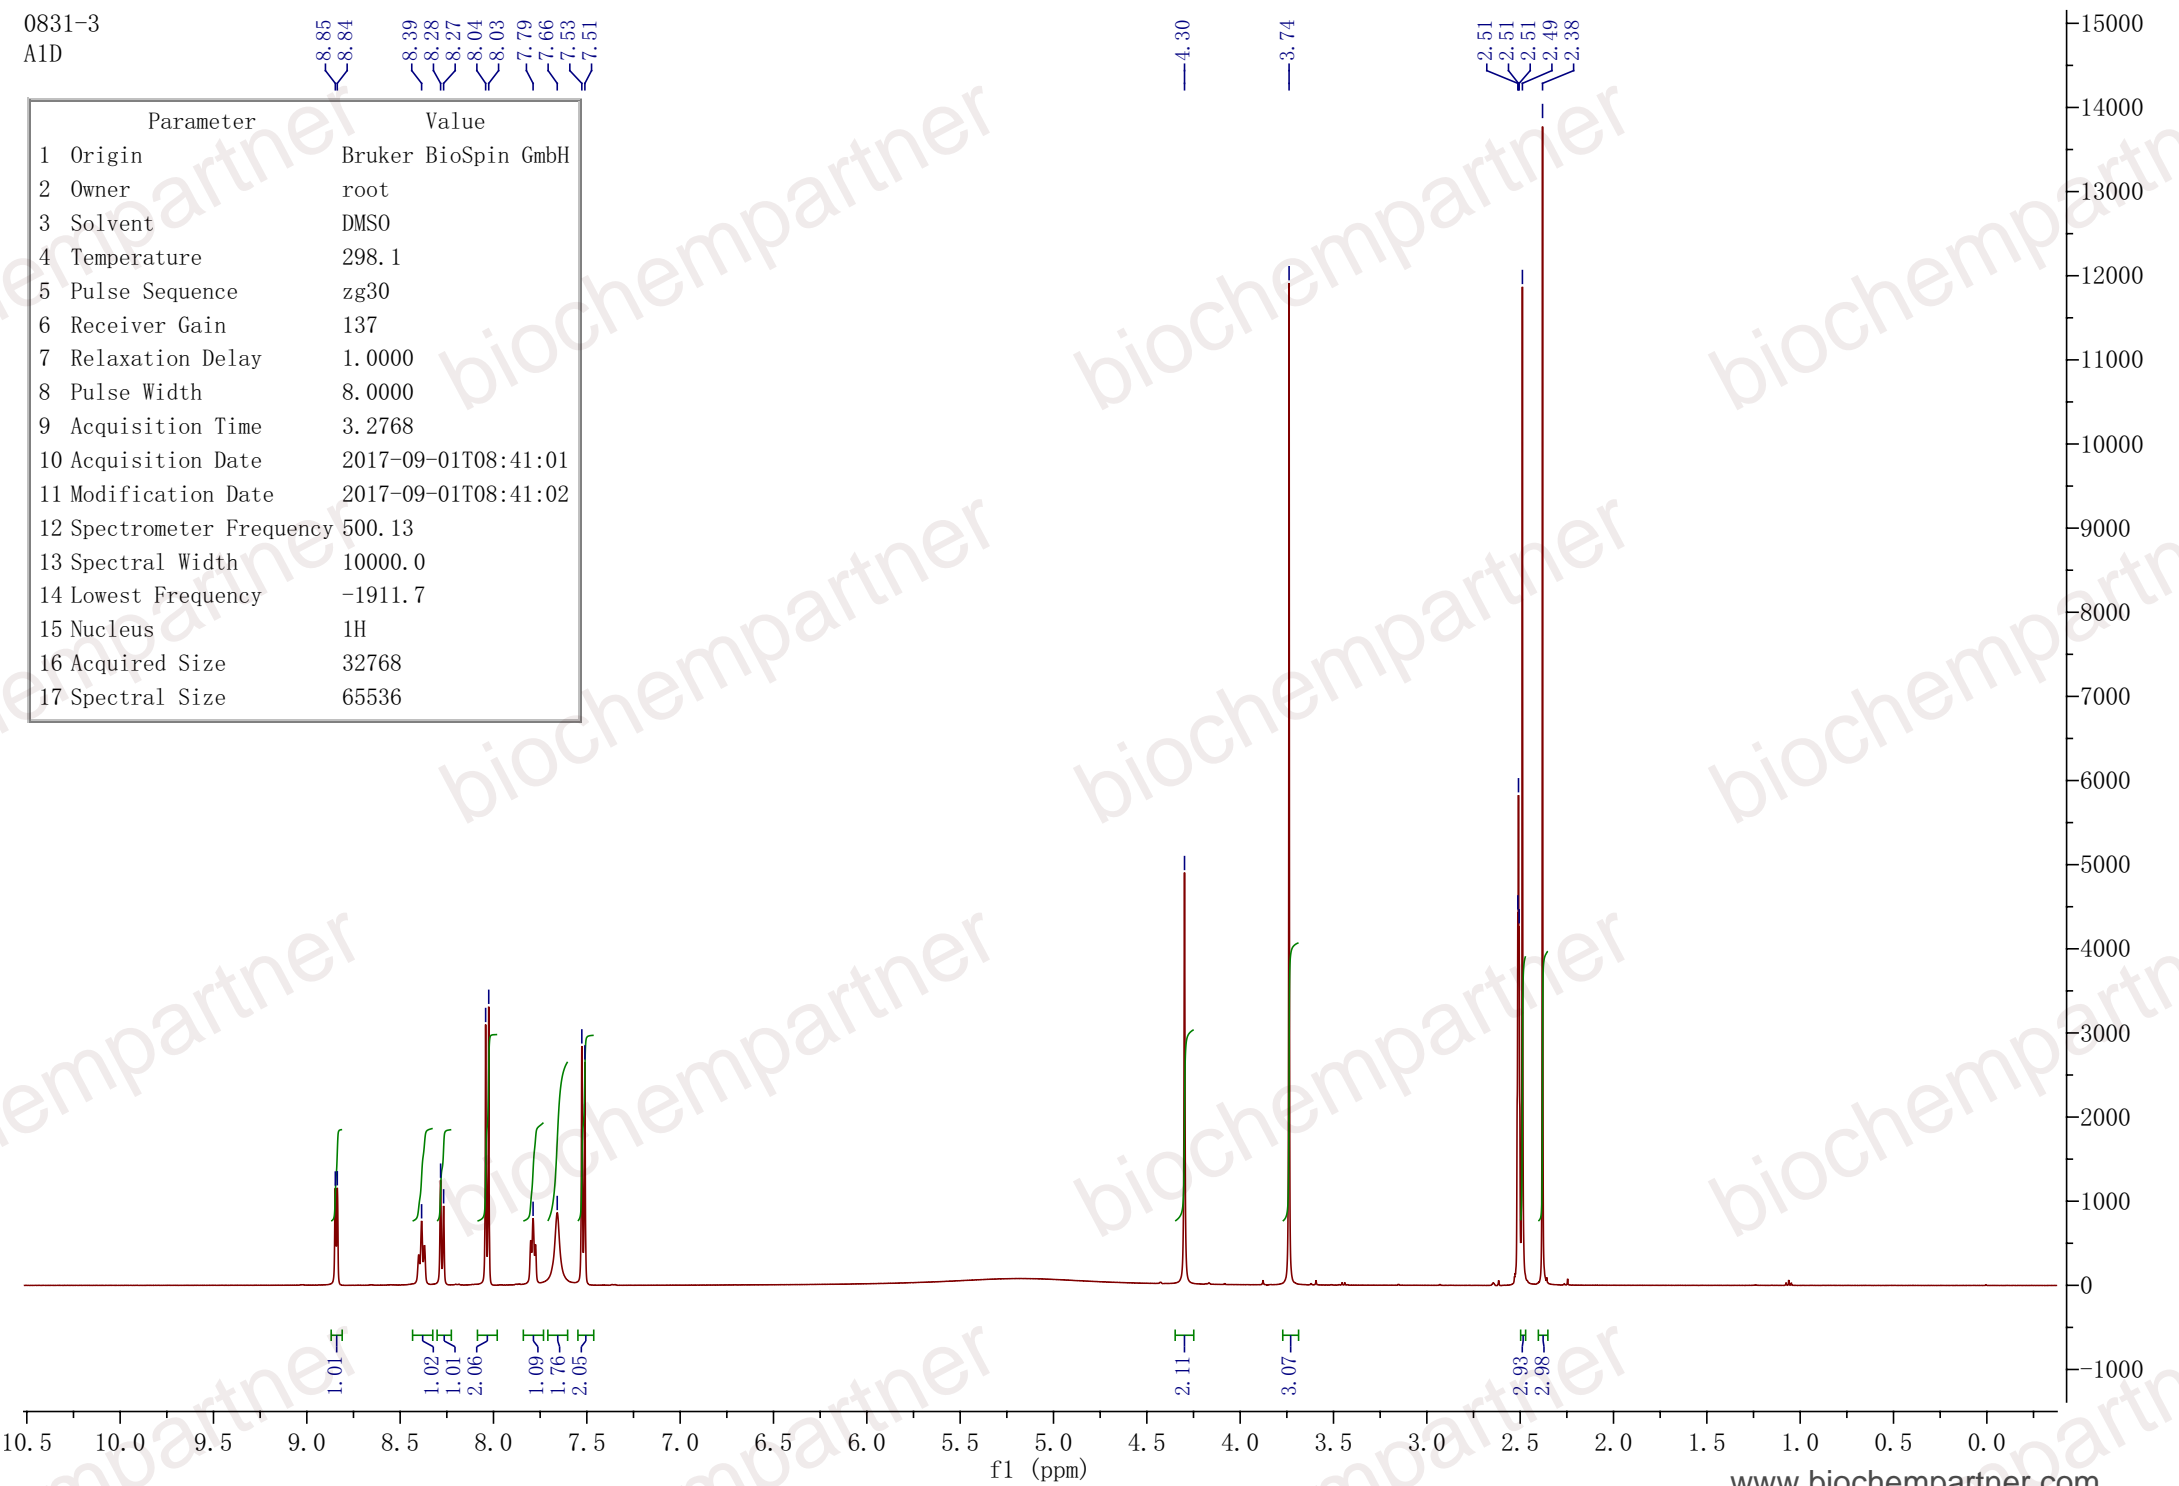

10.5 10.0 9.5 9.0 8.5 8.0 7.5 7.0 6.5 6.0 5.5 5.0 4.5 4.0 3.5 3.0 2.5 2.0 1.5 1.0 0.5 0.0

f1 (ppm)