


=====
Acq. Operator : Seq. Line : 1
Acq. Instrument : Instrument 1 Location : Vial 15
Injection Date : 4/17/2018 1:16:04 PM Inj : 1
Inj Volume : 3.0 µl
Different Inj Volume from Sequence ! Actual Inj Volume : 2.0 µl
Acq. Method : D:
Last changed : 3/24/2017 8:58:09 AM by 1
Analysis Method : D:\CHEM32\1\1.M
Last changed : 3/1/2018 2:26:59 PM
Sample Info : [A = ACN, B = 0.1% H3PO4/H2O] 0% A/B 2 min, 0-95% A/B 5 min, 95% A/B 3 min;
Athena C18 (3 µm, 2.1 mm * 100 mm); Flow: 0.45 ml/min, T = 25

Additional Info : Peak(s) manually integrated

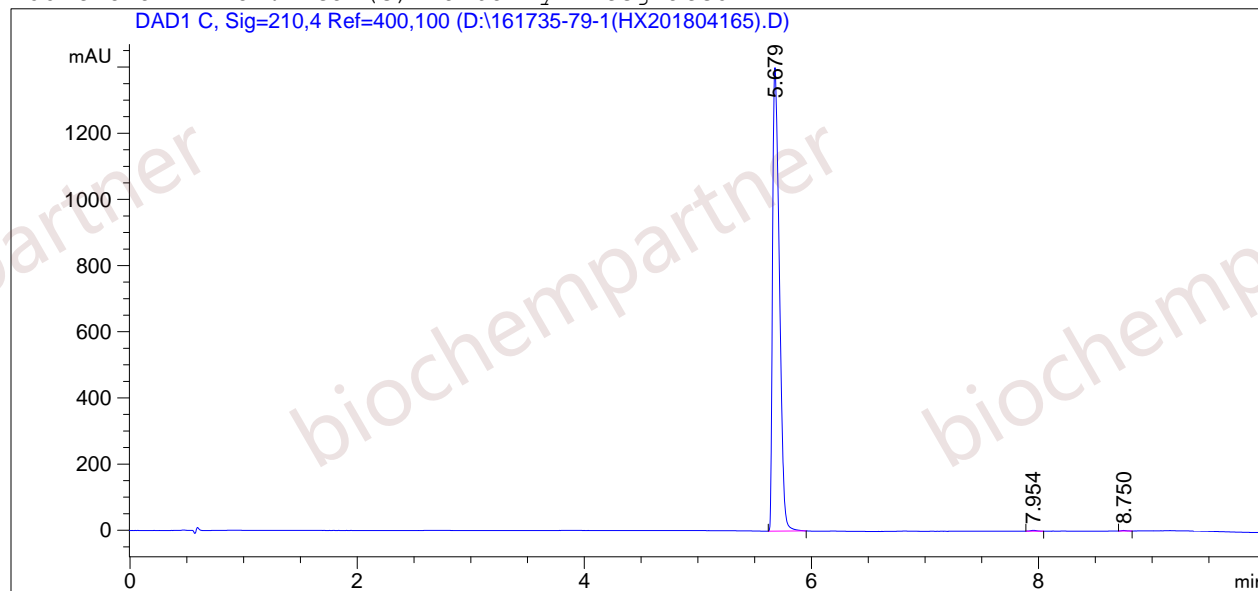

=====
Area Percent Report
=====

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: DAD1 C, Sig=210,4 Ref=400,100

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	5.679	BB	0.0661	5836.65820	1400.69958	99.7596
2	7.954	BB	0.0499	9.56383	2.66155	0.1635
3	8.750	BB	0.0373	4.50261	1.62841	0.0770
Totals :				5850.72464	1404.98954	

=====
*** End of Report ***