


Sample Name: BLANK

```

=====
Acq. Operator   : SYSTEM                      Seq. Line :    6
Acq. Instrument : Agilent HPLC                 Location  :   13
Injection Date  : 6/29/2018 3:10:53 PM       Inj       :    1
                                           Inj Volume: 5.000 µl
Different Inj Volume from Sample Entry! Actual Inj Volume : 1.000 µl
Acq. Method     : D:\2018\TEST\DATA\2018062\20180629-02 2018-06-29 13-18-11\5-(10)-100(5)-1-40-210.M
Last changed    : 6/29/2018 1:18:11 PM by SYSTEM
Analysis Method : D:\2018\TEST\DATA\2018062\20180629-02 2018-06-29 13-18-11\5-(10)-100(5)-1-40-210.M (Sequence Method)
Last changed    : 6/29/2018 3:36:11 PM by SYSTEM
                                           (modified after loading)
Additional Info : Peak(s) manually integrated
    
```

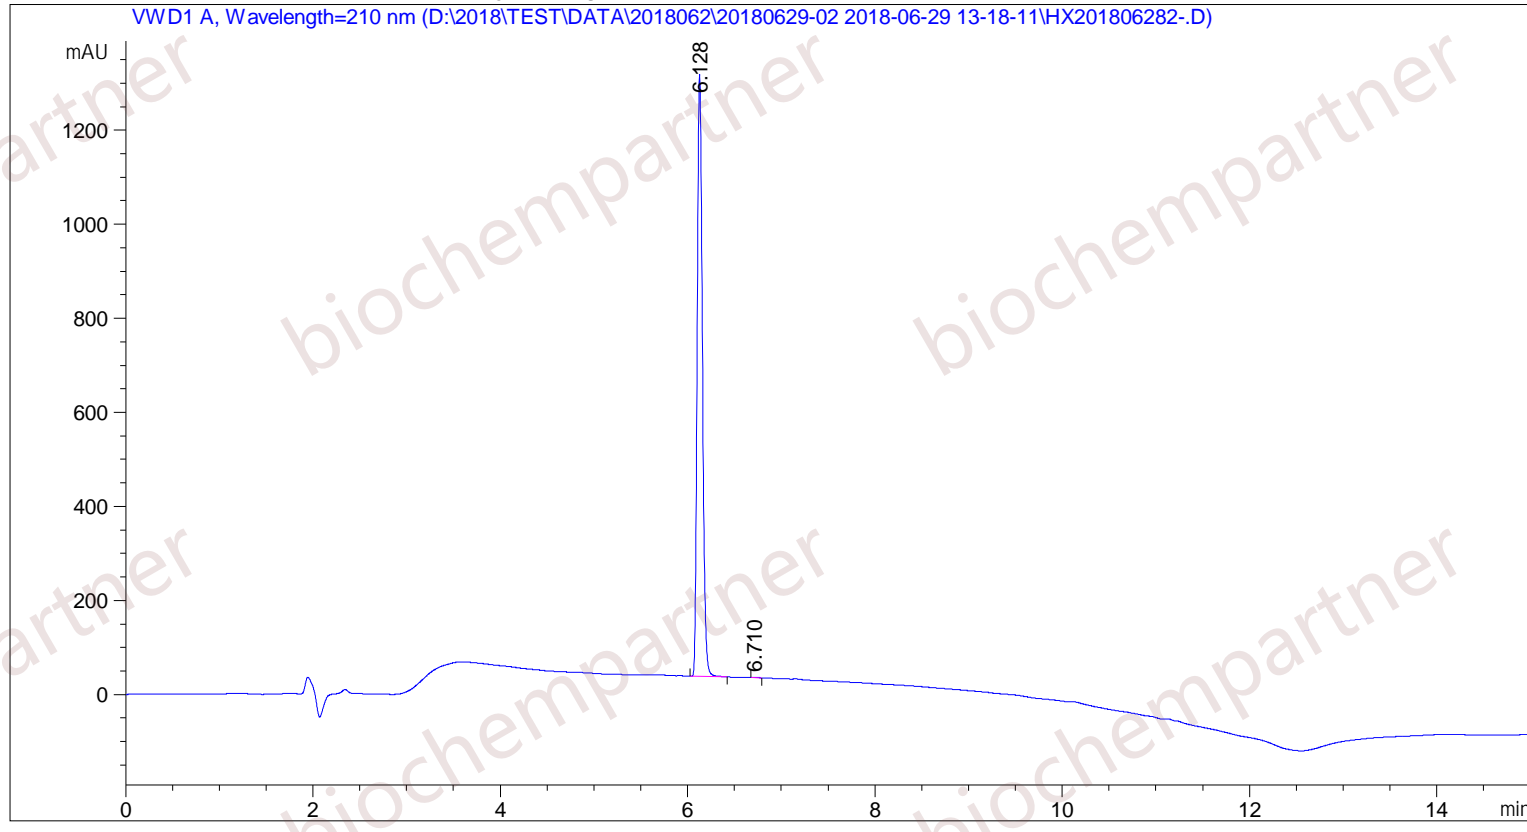

Area Percent Report

```

Sorted By      : Signal
Multiplier     : 1.0000
Dilution       : 1.0000
Use Multiplier & Dilution Factor with ISTDs
    
```

Signal 1: VWD1 A, Wavelength=210 nm

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	6.128	MM	0.0646	4970.36865	1281.94055	99.9726
2	6.710	MM	0.0647	1.36123	3.50854e-1	0.0274

Totals : 4971.72988 1282.29141

=====  
\*\*\* End of Report \*\*\*