


Sample Name: M-7-2-29

```

=====
Acq. Operator   : SYSTEM                               Seq. Line :    3
Acq. Instrument : Agilent HPLC                          Location  :   32
Injection Date  : 7/3/2018 9:57:37 AM                  Inj       :    1
                                                    Inj Volume: 5.000 µl
Different Inj Volume from Sample Entry! Actual Inj Volume : 0.500 µl
Acq. Method     : D:\2018\TEST\DATA\20180703\20180702-05 2018-07-03 09-08-44\5-(15)-100-210-40-1.M
Last changed    : 7/3/2018 9:08:44 AM by SYSTEM
Analysis Method : D:\2018\TEST\DATA\20180703\20180702-05 2018-07-03 09-08-44\5-(15)-100-210-40-1.M (Sequence Method)
Last changed    : 7/3/2018 10:20:48 AM by SYSTEM
                (modified after loading)
Additional Info : Peak(s) manually integrated
    
```

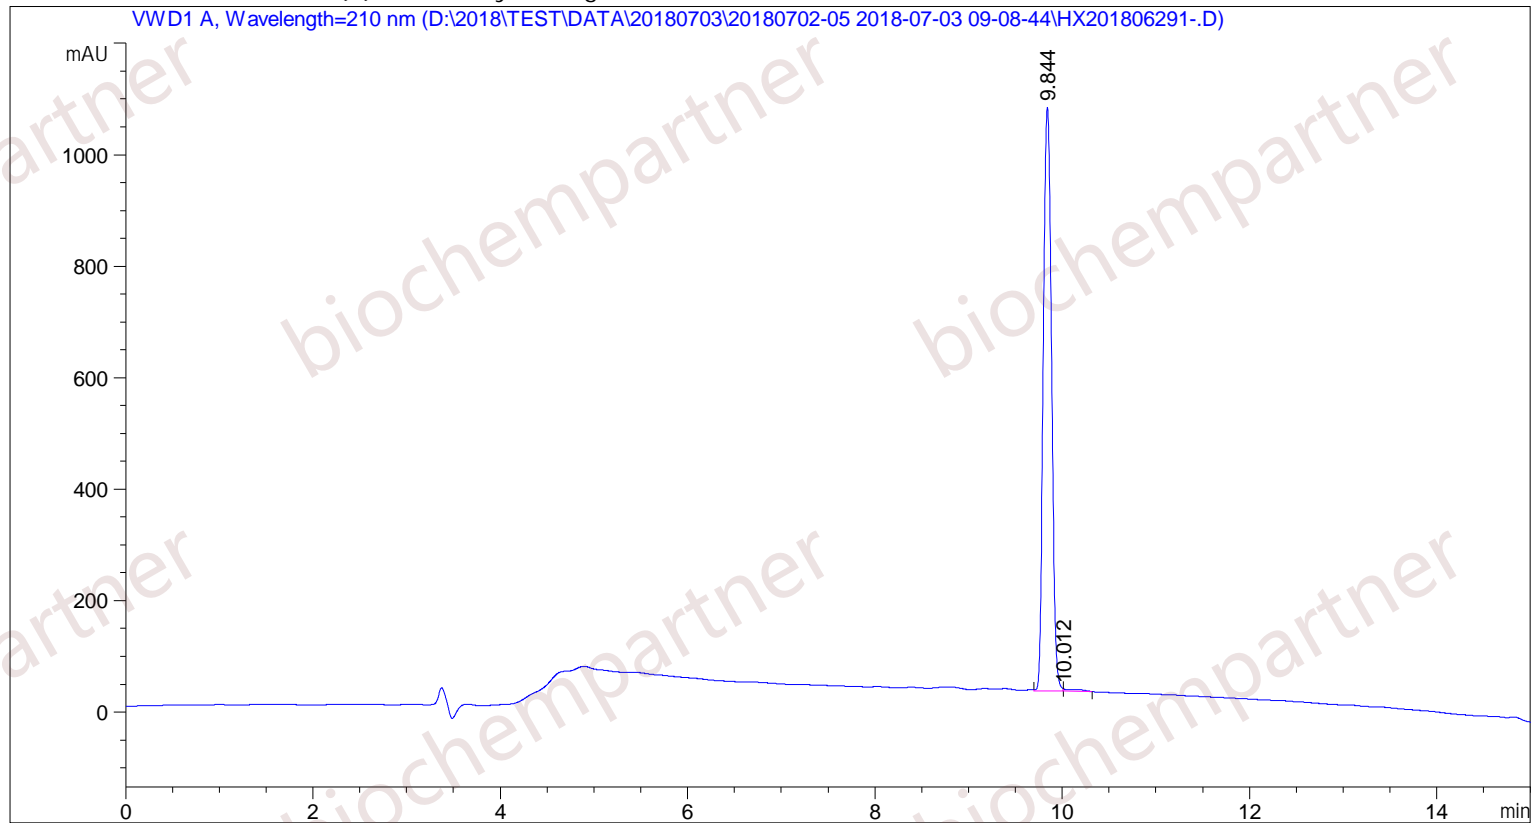

Area Percent Report

```

Sorted By      :      Signal
Multiplier     :      1.0000
Dilution       :      1.0000
Use Multiplier & Dilution Factor with ISTDs
    
```

Signal 1: VWD1 A, Wavelength=210 nm

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	9.844	MF	0.1015	6380.07471	1047.78174	99.4125
2	10.012	FM	0.1584	37.70417	4.04284	0.5875

Totals : 6417.77887 1051.82458

=====  
\*\*\* End of Report \*\*\*