


Parameter	Value
1 Comment	9D
2 Origin	Bruker BioSpin GmbH
3 Owner	root
4 Spectrometer	spect
5 Solvent	DMSO
6 Temperature	298.2
7 Pulse Sequence	zg30
8 Receiver Gain	61
9 Relaxation Delay	1.0000
10 Pulse Width	8.0000
11 Acquisition Time	3.2768
12 Acquisition Date	2018-04-20T16:19:11
13 Modification Date	2018-04-20T16:19:12
14 Spectrometer Frequency	500.13
15 Spectral Width	10000.0
16 Lowest Frequency	-1914.3
17 Nucleus	1H
18 Acquired Size	32768
19 Spectral Size	65536



=====
Acq. Operator : Seq. Line : 1
Acq. Instrument : Instrument 1 Location : Vial 38
Injection Date : 4/20/2018 12:49:43 PM Inj : 1
Inj Volume : 3.0 µl
Acq. Method : D:
Last changed : 3/24/2017 8:58:09 AM by 1
Analysis Method : D:\CHEM32\1\1.M
Last changed : 4/20/2018 1:01:48 PM
(modified after loading)
Sample Info : [A = ACN, B = 0.1% H3PO4/H2O] 0% A/B 2 min, 0-95% A/B 5 min, 95% A/B 3 min;
Athena C18 (3 µm, 2.1 mm * 100 mm); Flow: 0.45 ml/min, T = 25

Additional Info : Peak(s) manually integrated

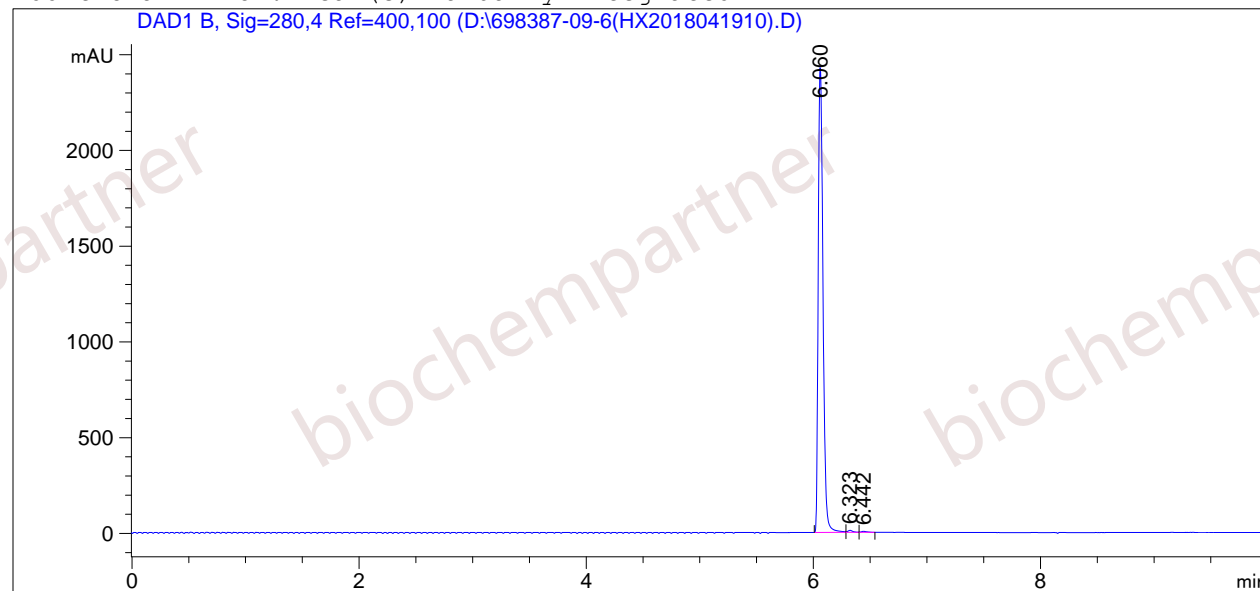

=====
Area Percent Report
=====

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: DAD1 B, Sig=280,4 Ref=400,100

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	6.060	BV	0.0460	7086.27393	2428.30371	99.2571
2	6.323	VV	0.0465	33.83079	10.66491	0.4739
3	6.442	VB	0.0480	19.20706	5.60815	0.2690
Totals :				7139.31178	2444.57677	

=====
*** End of Report ***