


LC/MS Report

File D:
 Injection Date : 8 Apr 14 6:14 pm +0800 Tgt Mass (EZX) :
 Sample Name : 1007207-67-1 2014040406 Location : P1-E-09
 Acq. Operator : Product Inj : 1
 Spec. Reported : MS Integration Inj Volume : 1 ul
 Acq. Method : D:\METHODS\1-POS-MON.M
 Analysis Method : D:\METHODS\1-POS-MON.M
 Sample Info : Easy-Access Method: '1-POS-MON'
 Method Info : Mobile Phase: A: water(10mMNH4HCO3) B: ACN
 Gradient: 5%B increase to 95%B within1.2min,
 95%B for 1.3min,back to 5%B within 0.01min.
 Flow Rate: 2 mL/min
 Column: XBridge, 3.5um, 50*4.6mm
 Oven Temperature: 50 C
 Mass Range:110-1000

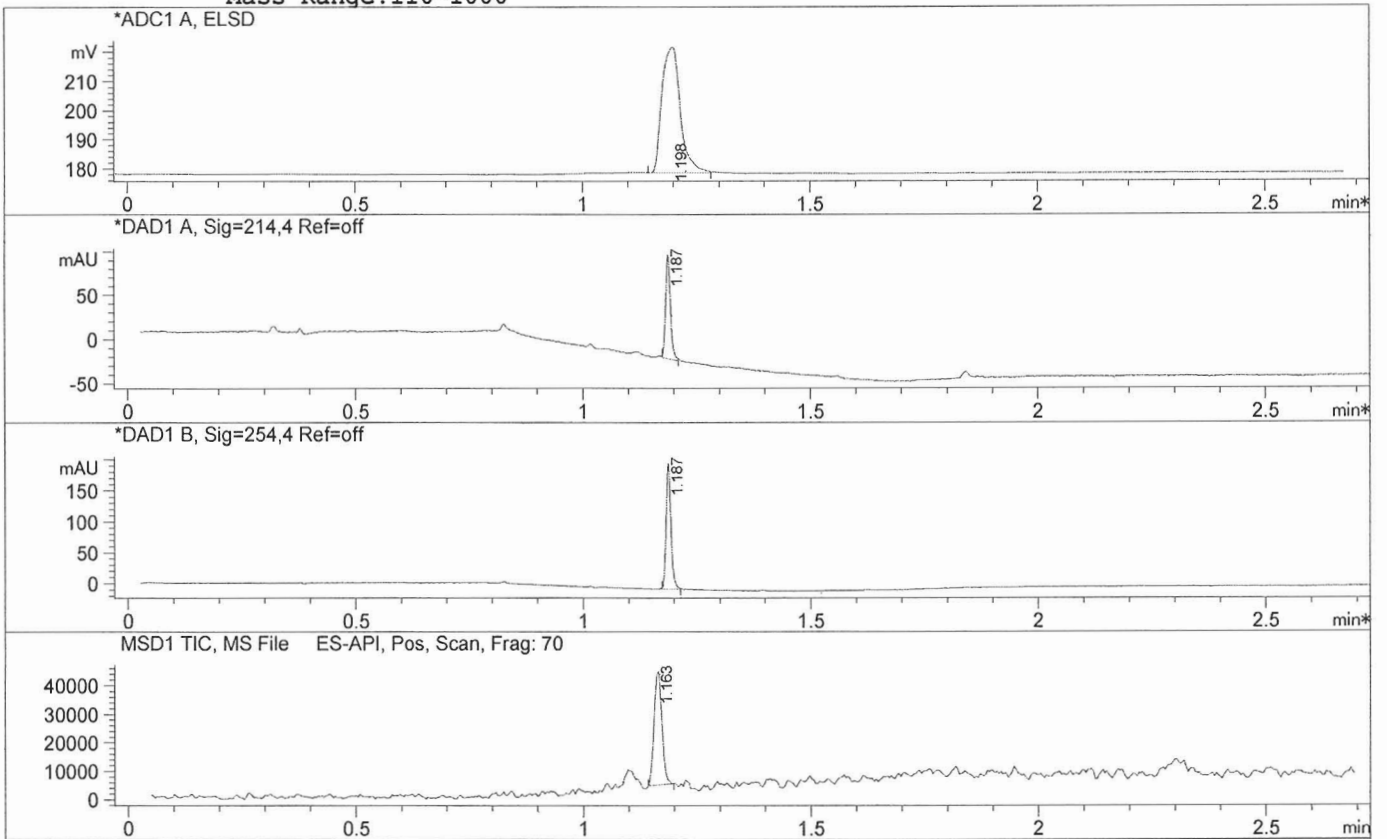

Integration Results for ADC1 A, ELSD

| RetTim | Width | Area | Height | Area% |
|--------|-------|--------|--------|--------|
| 1.20 | 0.05 | 120.24 | 43.08 | 100.00 |

Integration Results for DAD1 A, Sig=214,4 Ref=off

| RetTim | Width | Area | Height | Area% |
|--------|-------|-------|--------|--------|
| 1.19 | 0.01 | 86.82 | 119.12 | 100.00 |

Integration Results for DAD1 B, Sig=254,4 Ref=off

| RetTim | Width | Area | Height | Area% |
|--------|-------|--------|--------|--------|
| 1.19 | 0.01 | 149.49 | 204.03 | 100.00 |

LC/MS Report

Ret. Time: 1.16

<<<< POSITIVE SPECTRA >>>>

