



File D:\DATA\
Injection Date : 29 Mar 16 5:06 pm +0800 Tgt Mass(EZX) :
Sample Name : Location :
Acq. Operator : Inj : 1
Spec. Reported : MS Integration Inj Volume : 0.4 u1
Acq. Method : D:\METHODS\1-POS-3MIN.M
Analysis Method : D:\METHODS\1-POS-3MIN.M
Sample Info : Easy-Access Method: '1-POS-3MIN.M'
Method Info : Column:SUNFIRE C18 4.6X50mm,3.5um
Mobile phase: H2O(0.01%TFA) (A) / ACN(0.01% TFA)(B)
Elution program: Gradient from 5 to 95% of B in1.4min at 2.0ml/min
Temperature: 45°C
Detection: UV (214 , 4 nm) and MS (ESI, POS mode ,113 to 1200 amu)


*DAD1 A, Sig=214,4 Ref=off

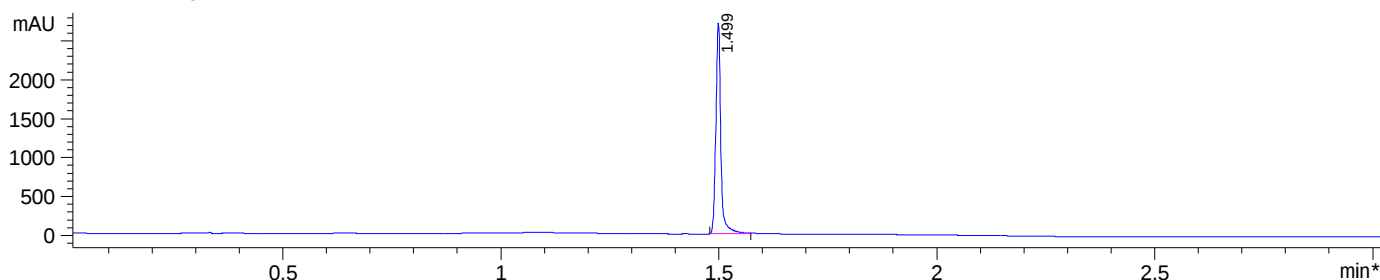

*DAD1 B, Sig=254,4 Ref=off

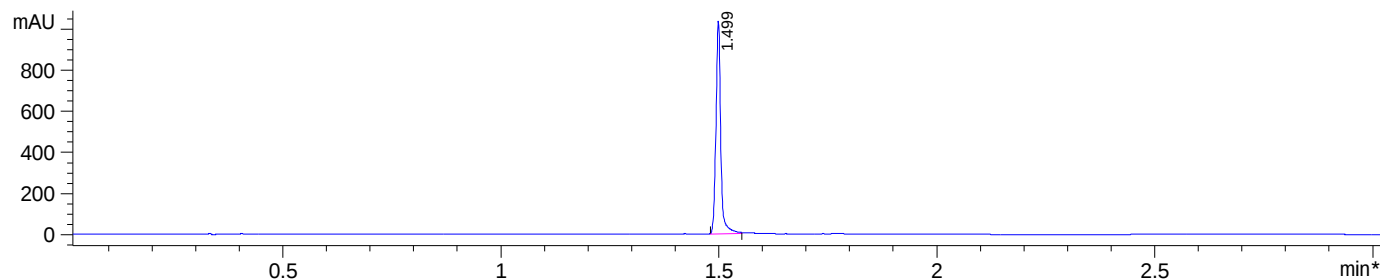

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 80

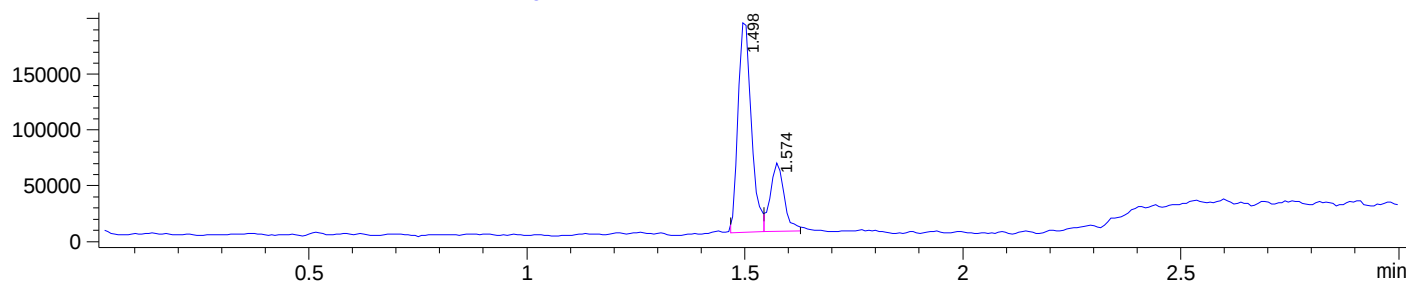

Integration Results for DAD1 A, Sig=214,4 Ref=off


RetTim	Width	Area	Height	Area%
1.50	0.01	2172.90	2702.09	100.00

Integration Results for DAD1 B, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%
1.50	0.01	797.96	1031.05	100.00

Ret. Time: 1.50

<<<< POSITIVE SPECTRA >>>>

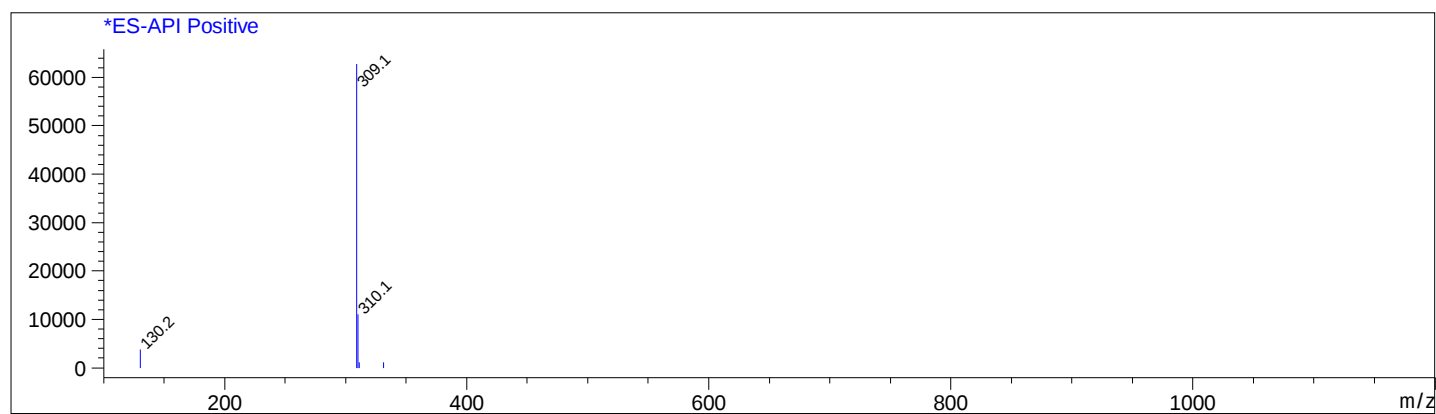

Ret. Time: 1.57

