



File D:\DATA\
 Injection Date : 7 Sep 16 2:47 pm +0800 Tgt Mass(EZX) :
 Sample Name : Location :
 Acq. Operator : Inj : 1
 Spec. Reported : MS Integration Inj Volume : 2 ul
 Acq. Method : D:\METHODS\1-POS-3MIN.M
 Analysis Method : D:\METHODS\1-POS-3MIN.M
 Sample Info : Easy-Access Method: '1-POS-3MIN'
 Method Info : Mobile Phase: A: Water(0.01%TFA) B: ACN(0.01%TFA)
 Gradient: 5%B increase to 95%B within 1.2min,
 95%B for 1.5min,back to 5%B within 0.01min.
 Flow Rate: 2.0 mL/min
 Column: SunFire C18, 4.6*50mm,3.5um
 Column Temperature: 40 C

Detection:UV(214,4nm) and MS(ESI,Pos mode,110 to 1100 amu)


*DAD1 A, Sig=214,4 Ref=off

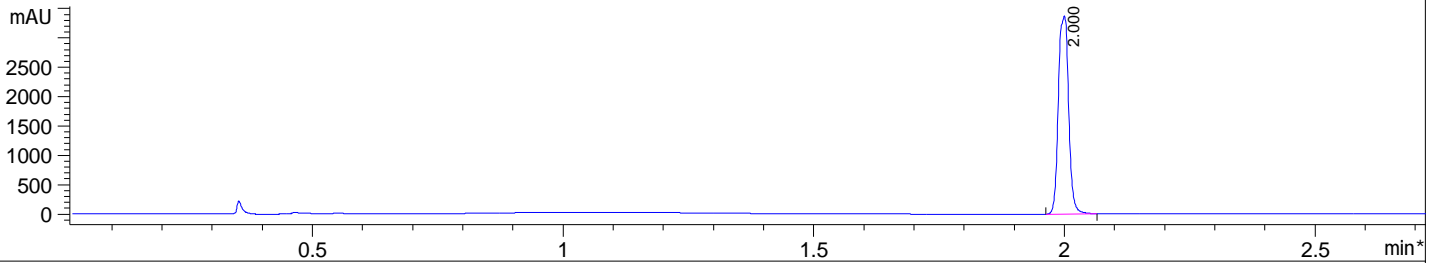

*DAD1 B, Sig=254,4 Ref=off

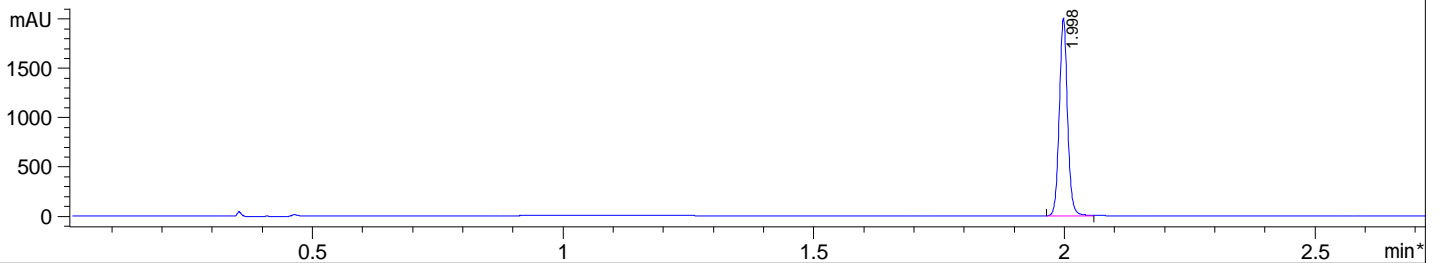

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 70

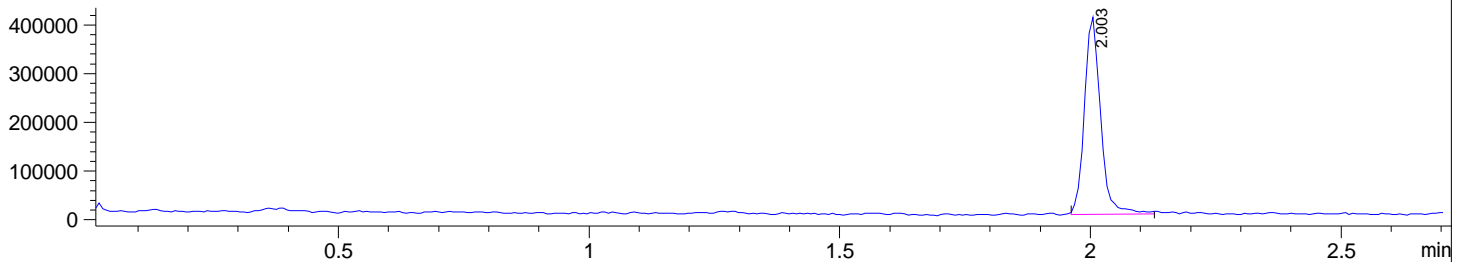

Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%
2.00	0.02	4818.88	3374.63	100.00

Integration Results for DAD1 B, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%
2.00	0.02	2285.37	2005.28	100.00

Ret. Time: 2.00 <<<< POSITIVE SPECTRA >>>>

