

File D:\DATA\

Tgt Mass (EZX):

Injection Date : 21 Apr 17 2:52 pm +0800

Seq. Line : 0

Sample Name :

Location :

Acq. Operator :

Inj : 1

Spec. Reported : MS Integration

Inj Volume : 1 ul

Acq. Method : D:\METHODS\2-POS-MON-1.M

Analysis Method : D:\METHODS\2-POS-MON-1.M

Sample Info : Easy-Access Method: '1-POS-MON-1'

Method Info : Column:Xbridge C18(2) (4.6x 50 mm, 3.5um)


Mobile phase: H2O(10 mmol NH4HCO3 ) (A) / ACN(B)

Elution program: Gradient from 10 to 95% of B in 1.5min at 1.8ml/min


Temperature: 50 °C

Detection: UV (214,254 nm) and MS (ESI, Pos mode ,103 to 800 amu)


\*DAD1 A, Sig=214,4 Ref=off

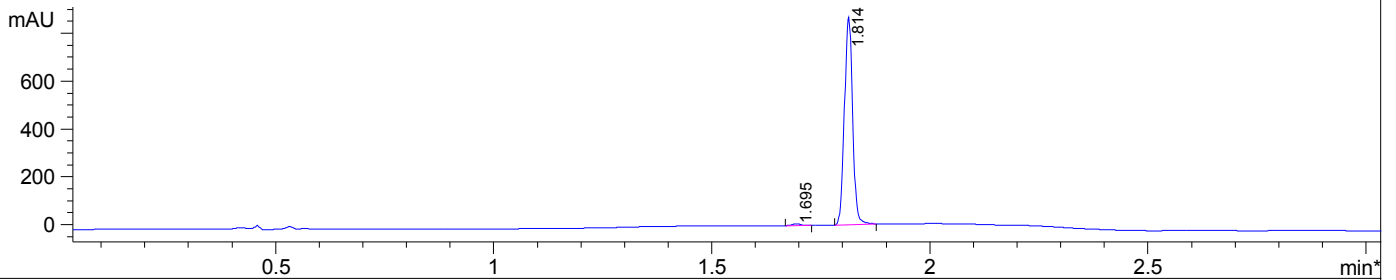

\*DAD1 B, Sig=254,4 Ref=off

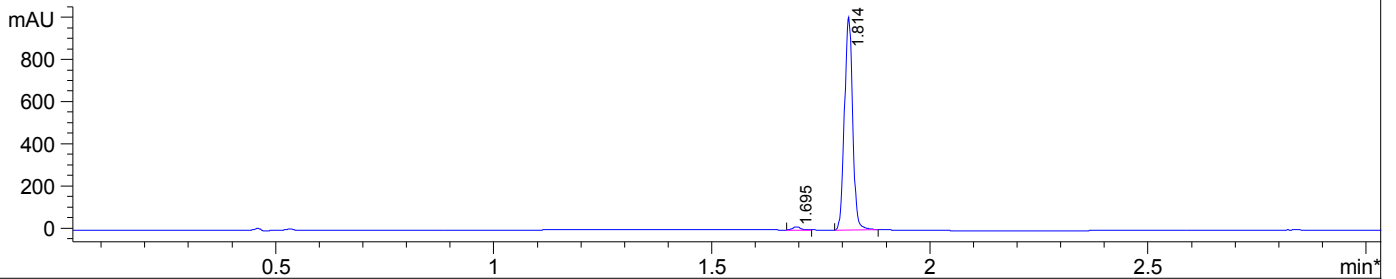

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 80

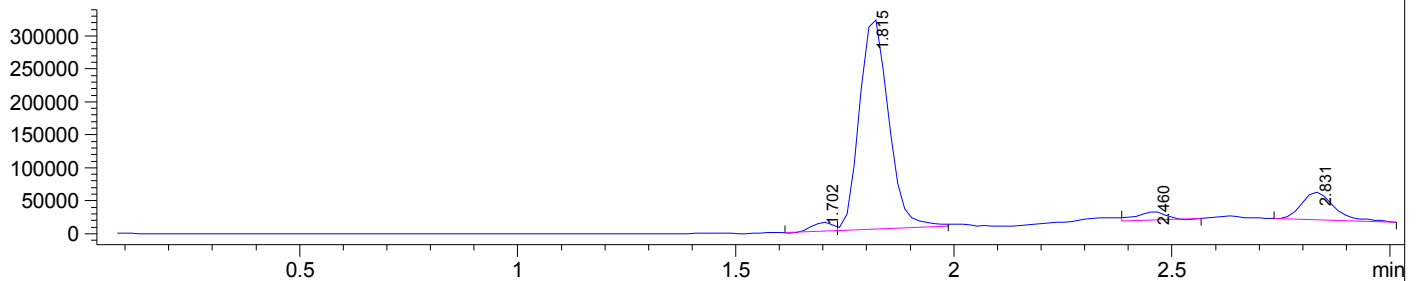

Integration Results for DAD1 A, Sig=214,4 Ref=off


RetTim	Width	Area	Height	Area%
1.69	0.02	9.90	7.89	0.87
1.81	0.02	1133.59	868.73	99.13

Integration Results for DAD1 B, Sig=254,4 Ref=off


RetTim	Width	Area	Height	Area%
1.69	0.02	19.28	15.15	1.44
1.81	0.02	1317.95	1010.76	98.56

Ret. Time: 1.70


&lt;&lt;&lt;&lt; POSITIVE SPECTRA &gt;&gt;&gt;&gt;

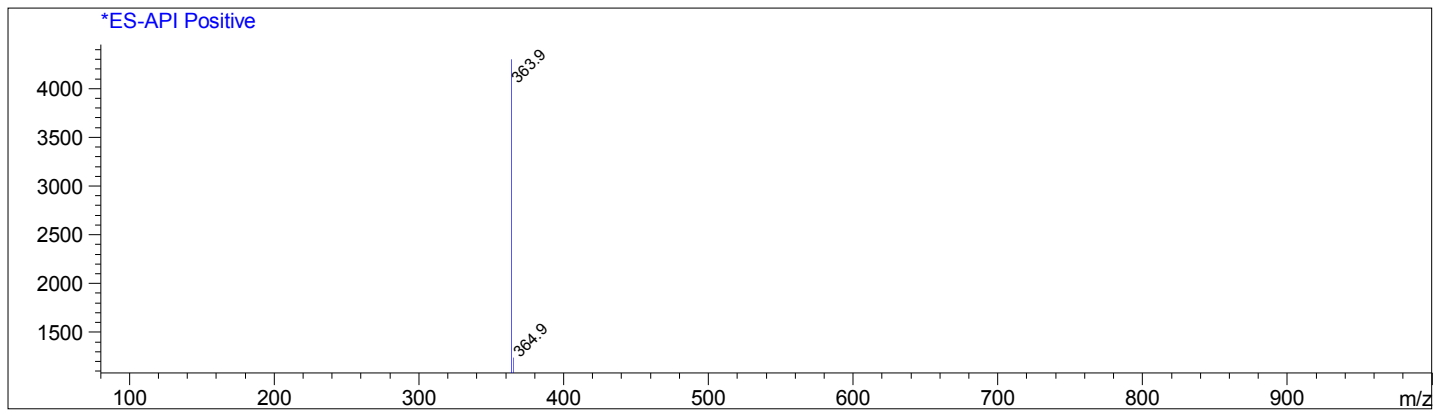

Ret. Time: 1.81

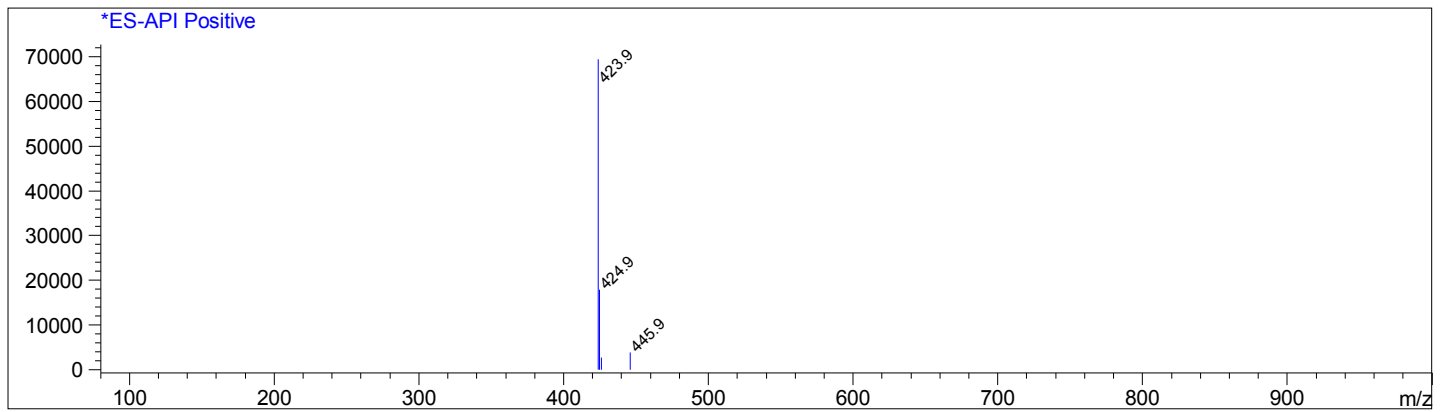

Ret. Time: 2.46

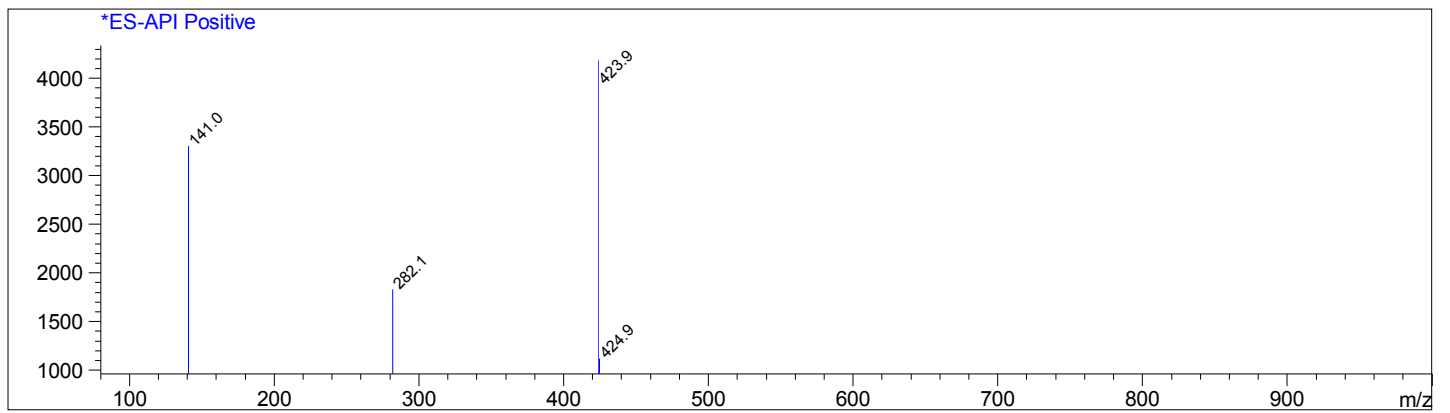

Ret. Time: 2.83

