

File D:\DATA\

Injection Date : 29-Dec-16, 17:50:51

Tgt Mass(EZX) :

Sample Name :

Location :

Acq. Operator :

Inj : 0

Spec. Reported : MS Integration

Inj Volume : 2 ul

Acq. Method : D:\METHODS\1-HPLC.M

Analysis Method : D:\METHODS\1-HPLC.M

Sample Info : Easy-Access Method: '1-HPLC'

Method Info : Mobile Phase: A: Water(0.01%TFA) B: ACN(0.01%TFA)


Gradient: 5%B increase to 95%B within 8min,
95%B for7min,back to 5%B within 0.01min.

Flow Rate: 1 mL/min


Column: SunFire C18, 4.6*150mm,3.5um

Column Temperature: 40 C

DAD1 A, Sig=214,4 Ref=off

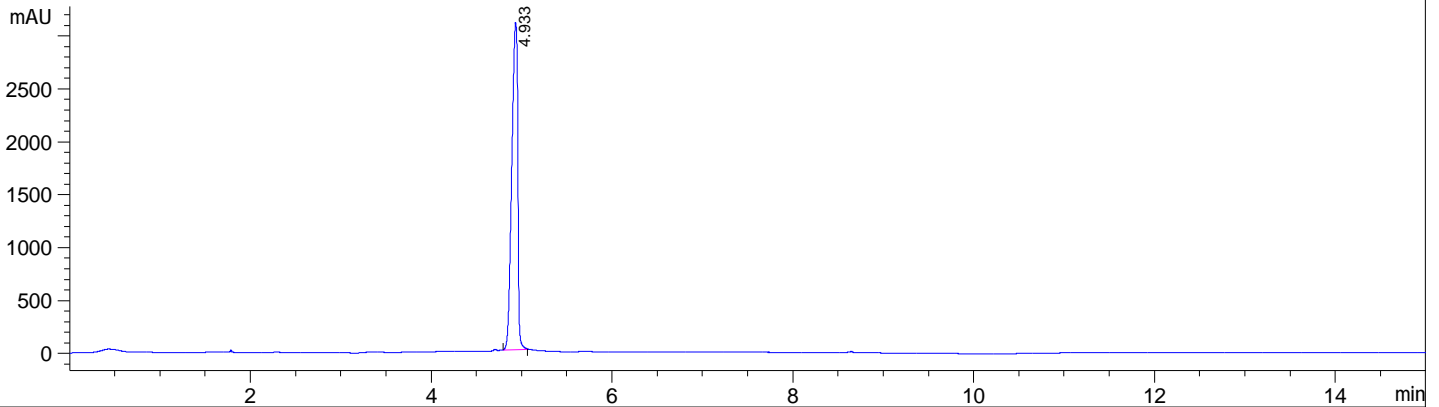

DAD1 B, Sig=254,4 Ref=off

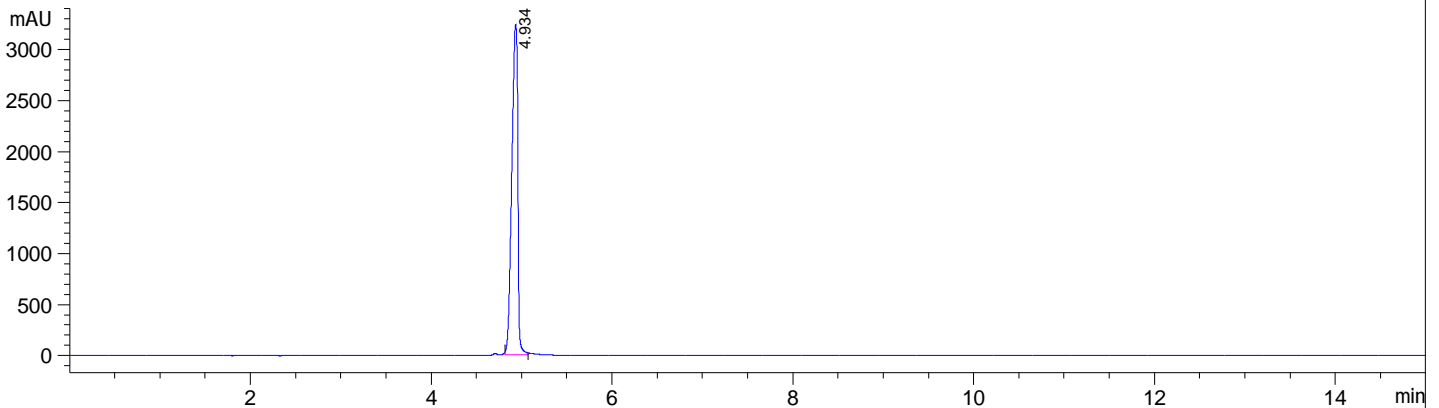

Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%
4.93	0.06	14279.07	3091.52	100.00

Integration Results for DAD1 B, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%
4.93	0.07	14973.56	3232.90	100.00