
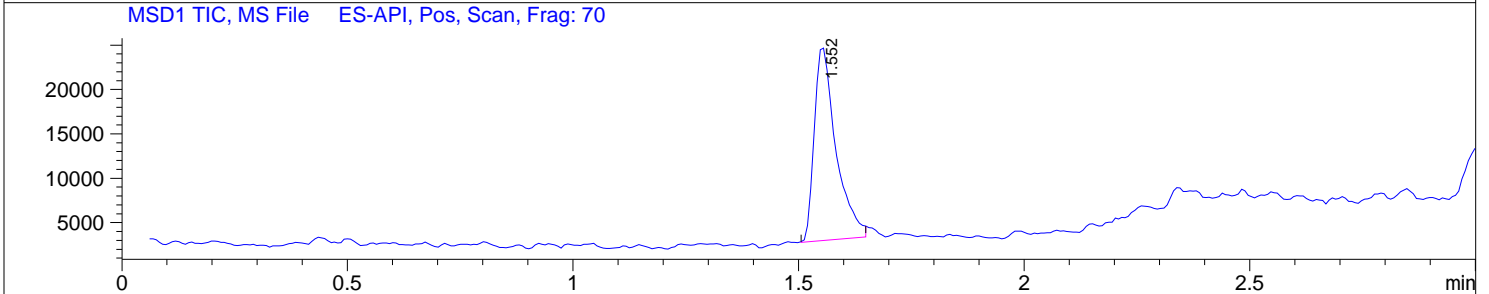
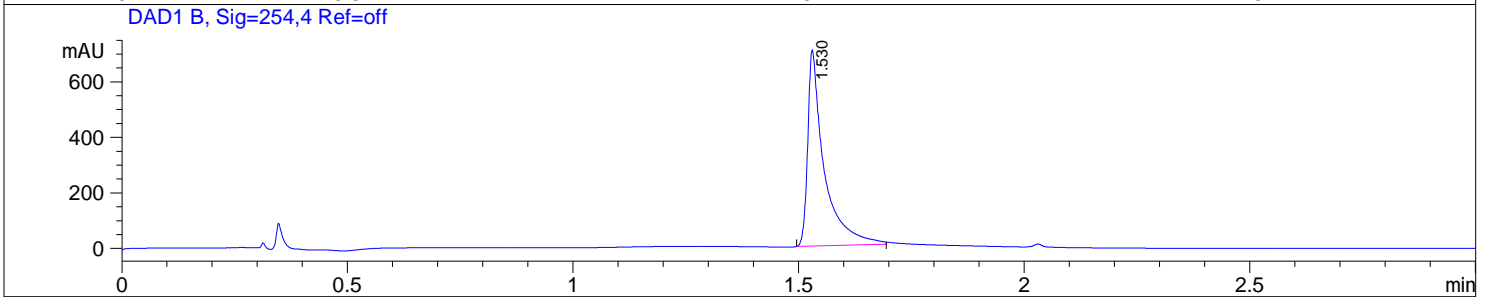


File D:\DATA\  
 Injection Date : 14 Feb 17 2:04 pm +0800 Tgt Mass(EZX) :  
 Sample Name : Location :  
 Acq. Operator : Inj : 1  
 Spec. Reported : MS Integration Inj Volume : 1 ul  
 Acq. Method : D:\METHODS\1-POS-3MIN.M  
 Analysis Method : D:\METHODS\1-POS-3MIN.M  
 Sample Info : Easy-Access Method: '1-POS-3MIN.M'  
 Method Info : Column:SUNFIRE C18 4.6X50mm,3.5um  
 Mobile phase: H2O(0.01%TFA) (A) / ACN(0.01% TFA)(B)  
 Elution program: Gradient from 5 to 95% of B in1.4min at 2.0ml/min  
 Temperature: 50°C  
 Detection: UV (214,254 nm) and MS (ESI, POS mode ,113 to 1200 amu)

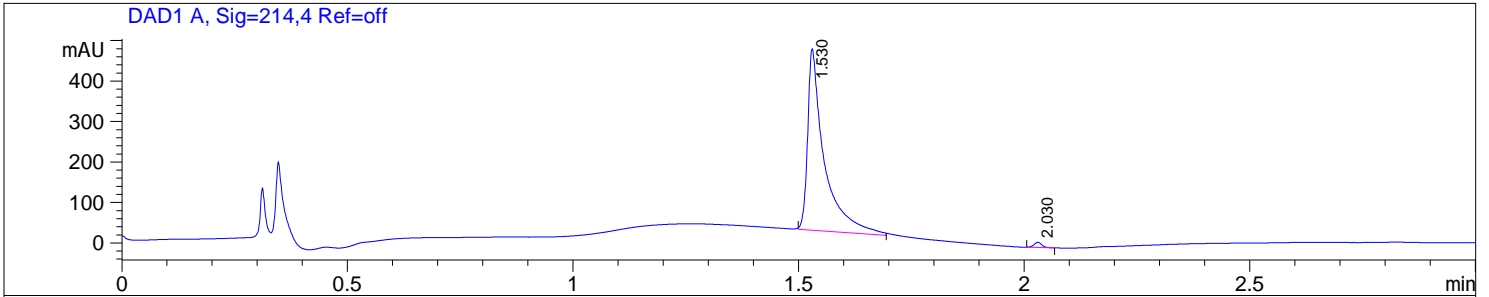

Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%
1.53	0.03	1144.58	447.81	98.66
2.03	0.02	15.50	13.00	1.34

Integration Results for DAD1 B, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%
1.53	0.03	1785.22	705.23	100.00

Ret. Time: 1.55

<<<< POSITIVE SPECTRA >>>>

