



File D:\DATA\
 Injection Date : 19-May-16, 18:52:17 Tgt Mass(EZX) :
 Sample Name : Location :
 Acq. Operator : Inj : 0
 Spec. Reported : MS Integration Inj Volume : 1 ul
 Acq. Method : D:\METHODS\1-HPLC.M
 Analysis Method : D:\METHODS\1-HPLC.M
 Sample Info : Easy-Access Method: '1-HPLC'
 Method Info : Mobile Phase: A: Water(0.01%TFA) B: ACN(0.01%TFA)
 Gradient: 5%B increase to 95%B within 8min,
 95%B for7min,back to 5%B within 0.01min.
 Flow Rate: 1 mL/min
 Column: SunFire C18, 4.6*150mm,3.5um
 Column Temperature: 40 C

DAD1 A, Sig=214,4 Ref=off

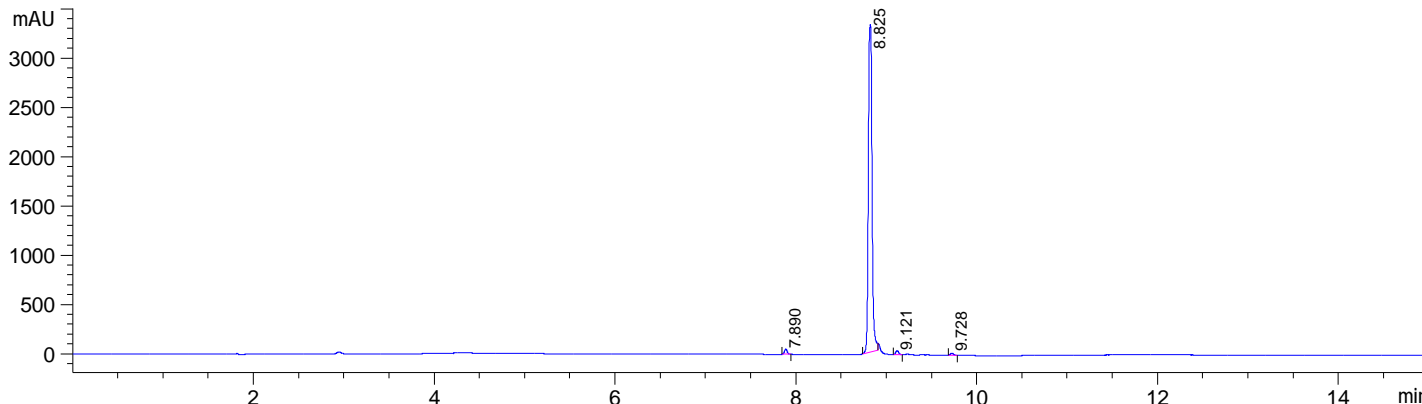

DAD1 B, Sig=254,4 Ref=off

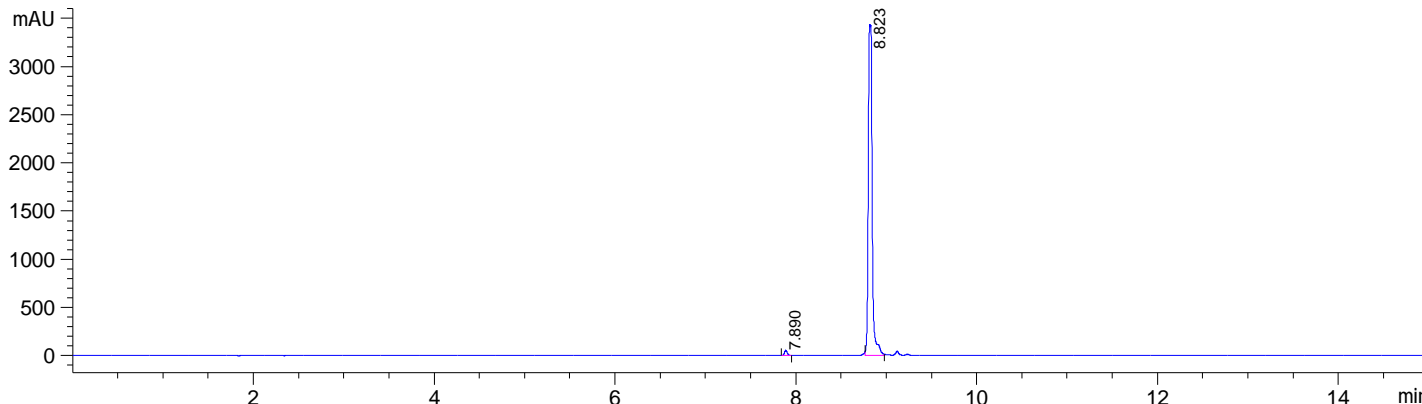

Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%
7.89	0.03	116.39	54.23	1.20
8.82	0.04	9424.66	3321.13	97.34
9.12	0.03	87.86	41.58	0.91
9.73	0.04	52.86	22.07	0.55

Integration Results for DAD1 B, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%
7.89	0.04	116.27	52.53	1.11
8.82	0.05	10380.06	3416.02	98.89