

File D:\DATA\

Tgt Mass (EZX):

Injection Date : 29 Dec 16 4:08 pm +0800

Seq. Line : 0

Sample Name :

Location :

Acq. Operator :

Inj : 1

Spec. Reported : MS Integration

Inj Volume : 3 ul

Acq. Method : D:\METHODS\2-POS-MON-1.M

Analysis Method : D:\METHODS\2-POS-MON-1.M

Sample Info : Easy-Access Method: '1-POS-MON-1'

Method Info : Column:Xbridge C18(2) (4.6x 50 mm, 3.5um)


Mobile phase: H2O(10 mmol NH4HCO3 ) (A) / ACN(B)

Elution program: Gradient from 10 to 95% of B in 1.5min at 1.8ml/min


Temperature: 50 °C

Detection: UV (214,254 nm) and MS (ESI, Pos mode ,103 to 800 amu)


\*DAD1 A, Sig=214,4 Ref=off

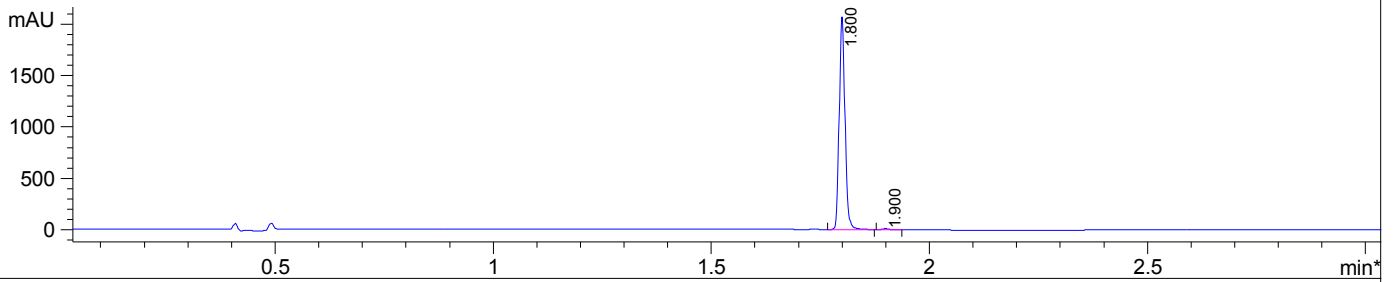

\*DAD1 B, Sig=254,4 Ref=off

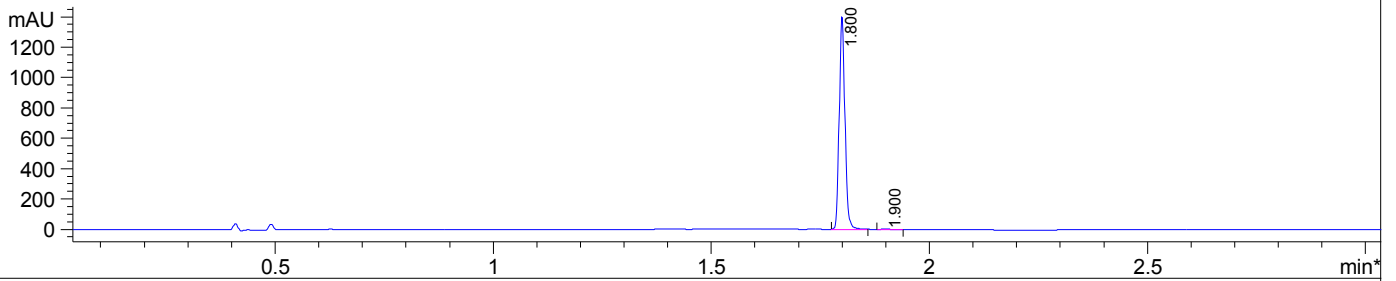

MSD1 TIC, MS File ES-API, Pos, Scan, Frag: 80

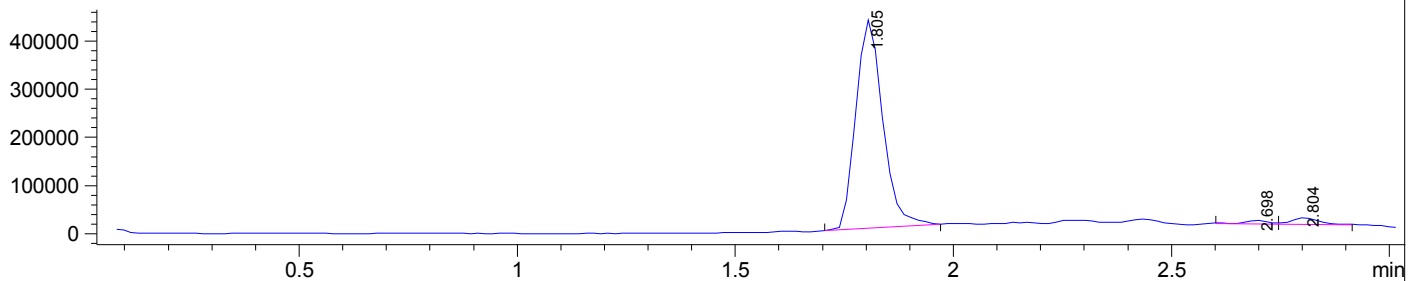

Integration Results for DAD1 A, Sig=214,4 Ref=off


RetTim	Width	Area	Height	Area%
1.80	0.01	1940.57	2086.60	99.29
1.90	0.02	13.91	12.29	0.71

Integration Results for DAD1 B, Sig=254,4 Ref=off


RetTim	Width	Area	Height	Area%
1.80	0.01	1294.55	1409.94	99.50
1.90	0.02	6.53	5.79	0.50

Ret. Time: 1.81

<<<< POSITIVE SPECTRA >>>>

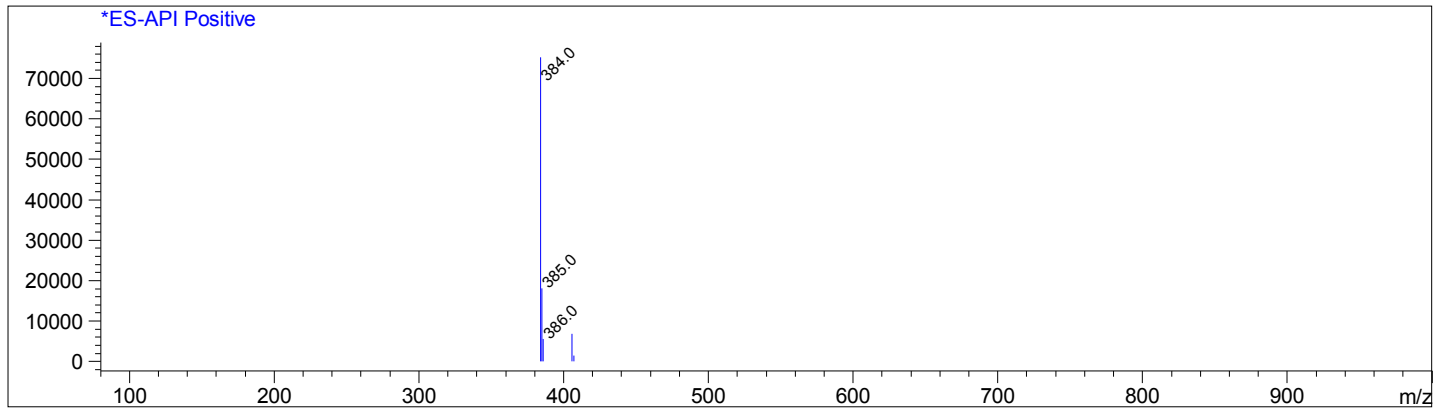

Ret. Time: 2.70

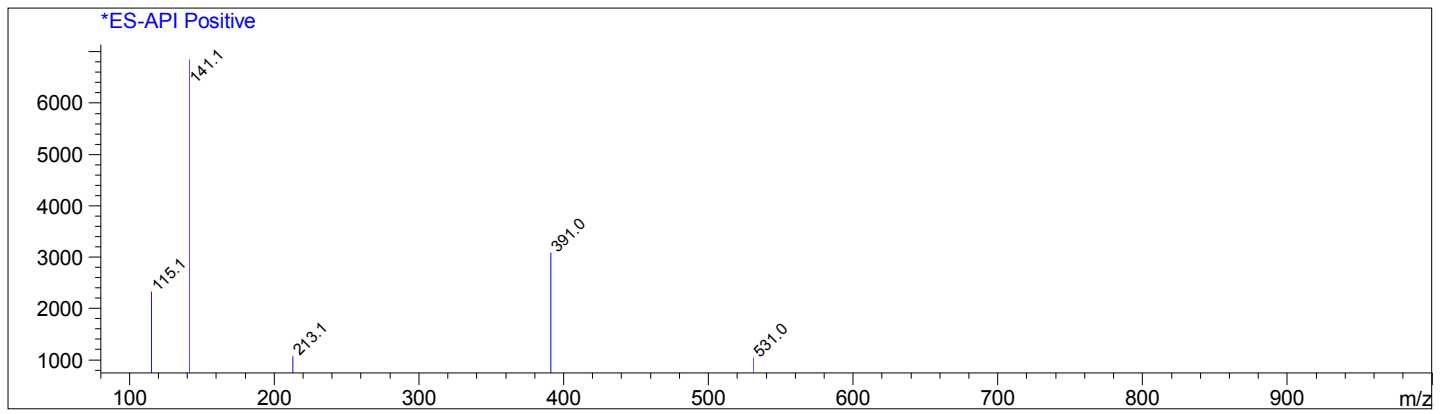

Ret. Time: 2.80

