
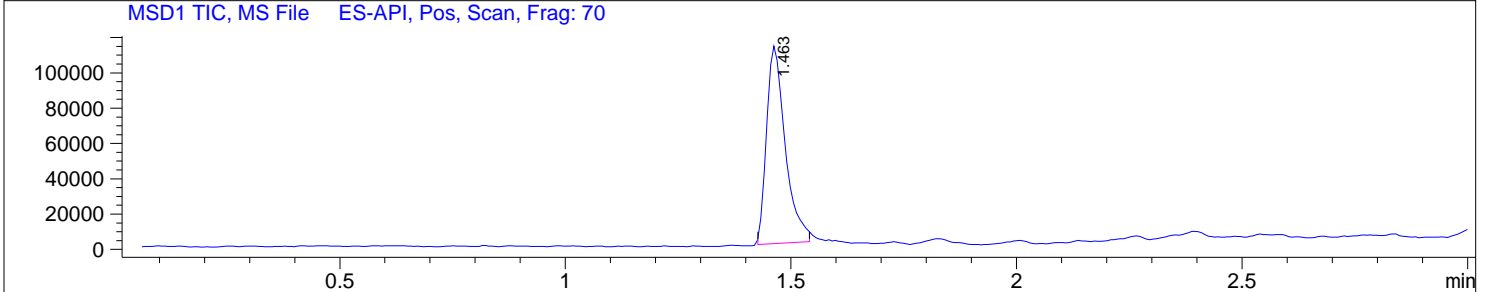
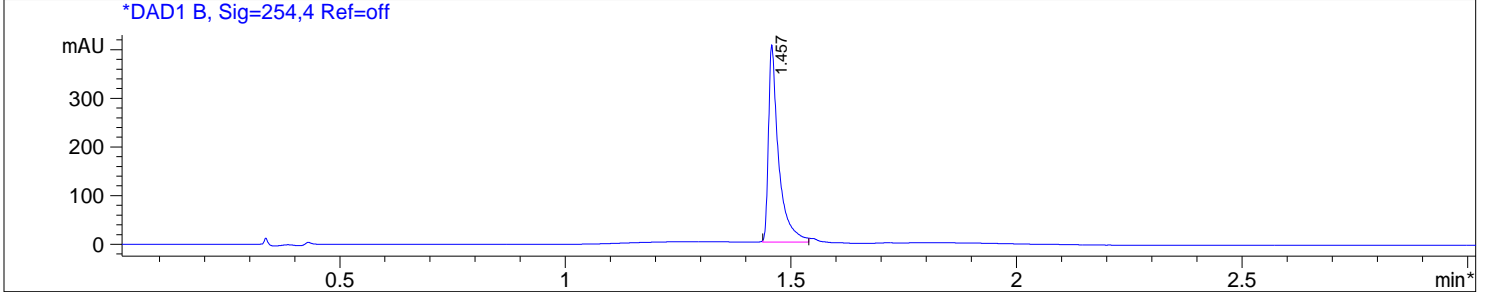


File D:\DATA\
 Injection Date : 15 Feb 17 1:14 pm +0800 Tgt Mass(EZX) :
 Sample Name : Location :
 Acq. Operator : Inj : 1
 Spec. Reported : MS Integration Inj Volume : 1 ul
 Acq. Method : D:\METHODS\1-POS-3MIN.M
 Analysis Method : D:\METHODS\1-POS-3MIN.M
 Sample Info : Easy-Access Method: '1-POS-3MIN.M'
 Method Info : Column:SUNFIRE C18 4.6X50mm,3.5um
 Mobile phase: H2O(0.01%TFA) (A) / ACN(0.01% TFA)(B)
 Elution program: Gradient from 5 to 95% of B in1.4min at 2.0ml/min
 Temperature: 50°C
 Detection: UV (214, 254 nm) and MS (ESI, POS mode ,113 to 1200 amu)

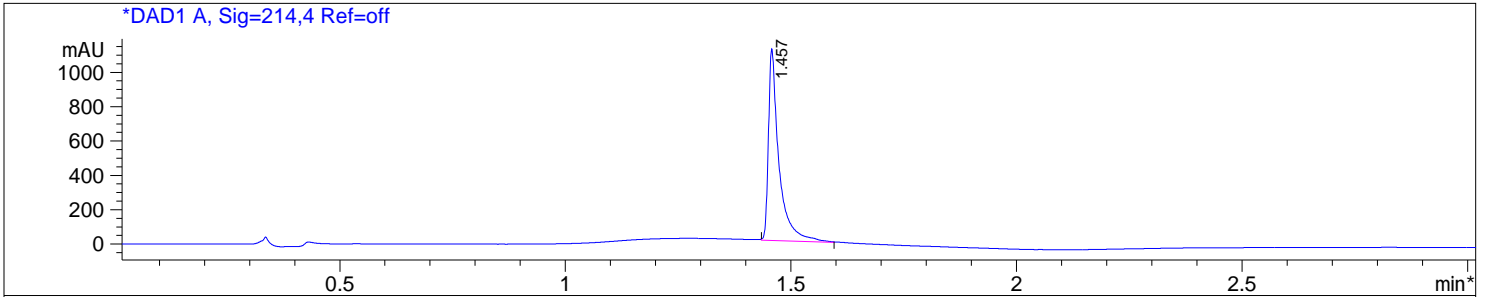

Integration Results for DAD1 A, Sig=214,4 Ref=off

| RetTim | Width | Area | Height | Area% |
|--------|-------|---------|---------|--------|
| 1.46 | 0.02 | 1806.41 | 1114.74 | 100.00 |

Integration Results for DAD1 B, Sig=254,4 Ref=off

| RetTim | Width | Area | Height | Area% |
|--------|-------|--------|--------|--------|
| 1.46 | 0.02 | 632.34 | 404.65 | 100.00 |

Ret. Time: 1.46

<<<< POSITIVE SPECTRA >>>>

