



File D:\DATA\  
 Injection Date : 08-Aug-16, 18:00:11 Tgt Mass(EZX) :  
 Sample Name : Location :  
 Acq. Operator : Inj : 0  
 Spec. Reported : MS Integration Inj Volume : 1 ul  
 Acq. Method : D:\METHODS\1-HPLC.M  
 Analysis Method : D:\METHODS\1-HPLC.M  
 Sample Info : Easy-Access Method: '1-HPLC'  
 Method Info : Mobile Phase: A: Water(0.01%TFA) B: ACN(0.01%TFA)  
 Gradient: 5%B increase to 95%B within 8min,  
 95%B for7min,back to 5%B within 0.01min.  
 Flow Rate: 1 mL/min  
 Column: SunFire C18, 4.6\*150mm,3.5um  
 Column Temperature: 40 C

DAD1 A, Sig=214,4 Ref=off

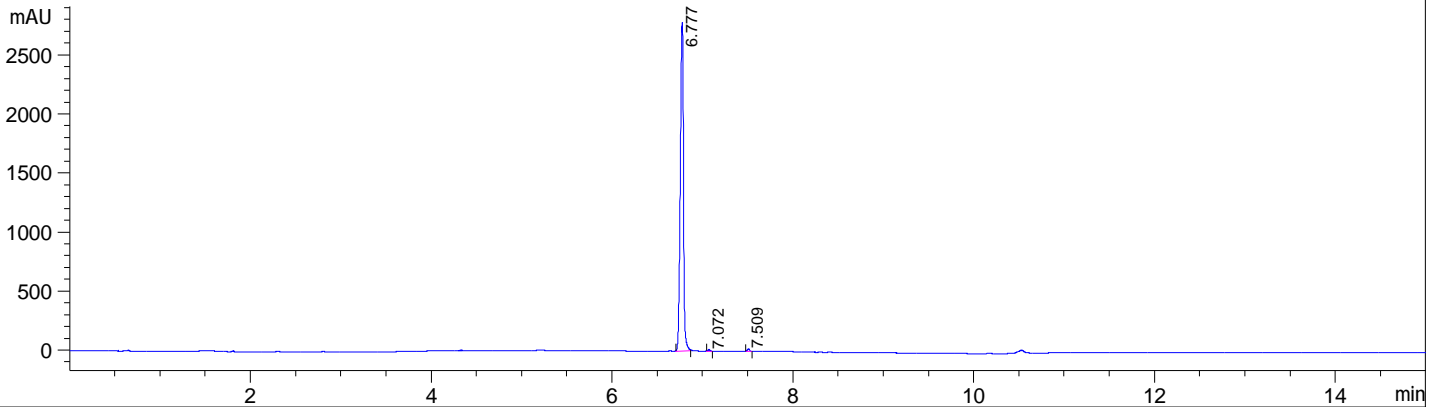

DAD1 B, Sig=254,4 Ref=off

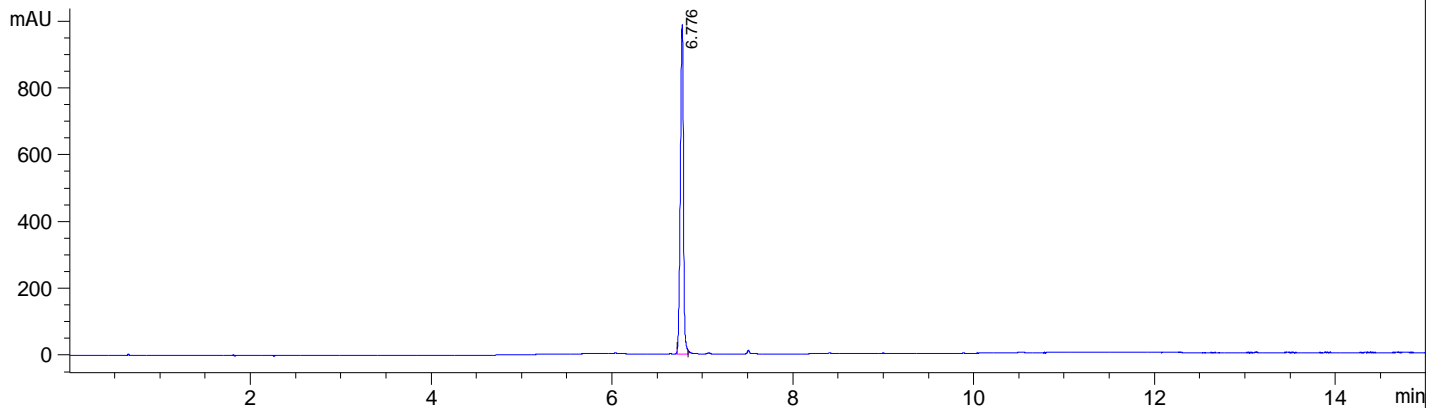

Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%
6.78	0.04	6837.23	2780.14	99.20
7.07	0.02	20.75	13.03	0.30
7.51	0.02	34.20	21.62	0.50

Integration Results for DAD1 B, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%
6.78	0.04	2360.81	981.40	100.00