


File D:\DATA
Injection Date : 20 Oct 14 2:45
Sample Name : 905854-02-6
Acq. Method : C:\Chem32\1\METHODS\1-POS-2MIN.M
Analysis Method : C:\Chem32\1\METHODS\1-POS-2MIN.M
Sample Info : Easy-Access Method: '1-POS-2MIN'
Method Info : Mobile Phase: A: Water(0.01%TFA) B: ACN(0.01%TFA)
Gradient: 5%B increase to 100%B within 0.8min,100%B for 1.1min.
Flow Rate:1.5mL/min
Column: Chromolith Fast Gradien RP-18e,50-3mm.
Column Temperature: 40C
Mass Range:100-1100

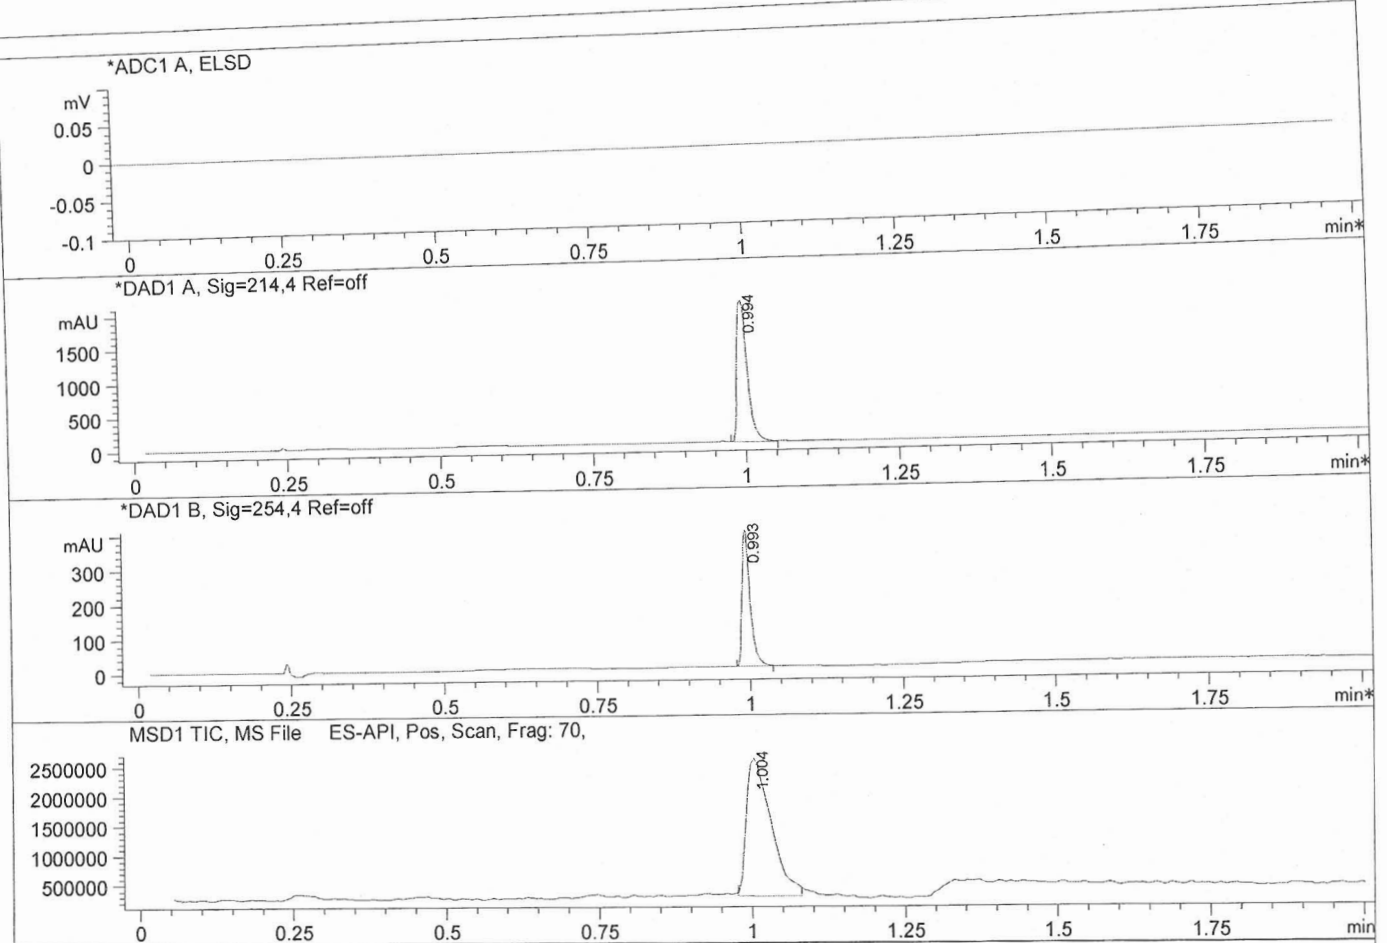

Integration Results for ADC1 A, ELSD

RetTim	Width	Area	Height	Area%
0.99	0.02	2385.59	2026.89	100.00

Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%
0.99	0.02	2385.59	2026.89	100.00

Integration Results for DAD1 B, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%
0.99	0.01	354.72	386.71	100.00

LC/MS Report

Ret. Time: 1.00 <<<< POSITIVE SPECTRA >>>>

