



File D:\DATA

Acq. Method : C:\Chem32\1\METHODS\2-HPLC-15MIN.M
Analysis Method : C:\Chem32\1\METHODS\2-HPLC-15MIN.M
Sample Info : *** No target masses specified ***
Method Info : Mobile Phase: A: water(0.01%TFA) B: ACN(0.01%TFA)
Gradient: 0min 5%B,3min 5%B,10min 95%B,15min 95%B
Flow Rate: 1.2 ml/min
Column: Eclipse XDB-C18,4.6*150mm,5um
Oven Temperature: 40 C


ADC1 A, ELSD

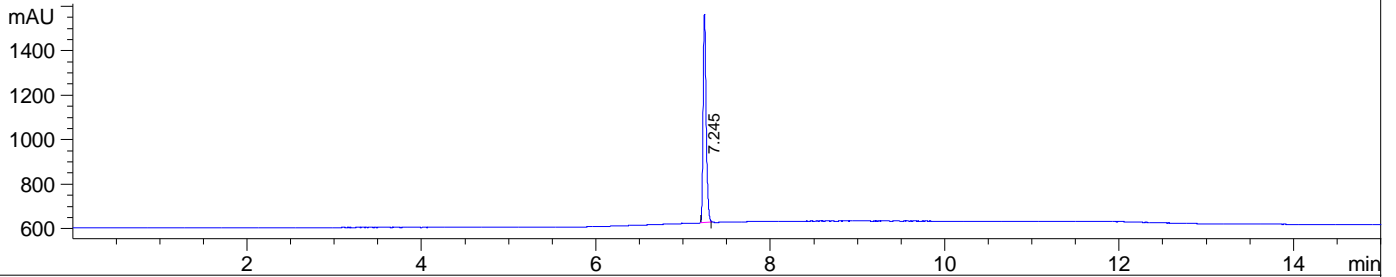

DAD1 A, Sig=214,4 Ref=off

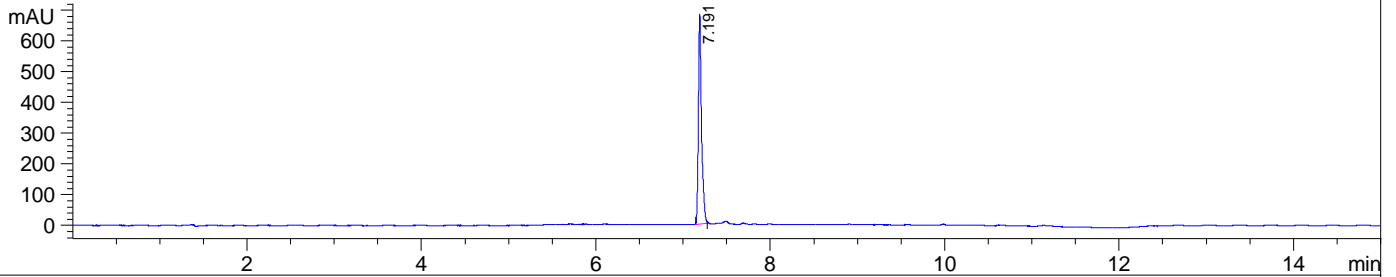

DAD1 B, Sig=254,4 Ref=off

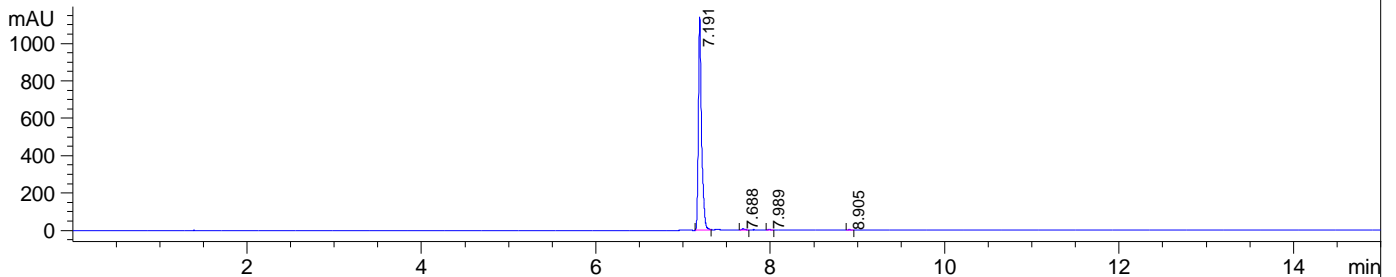

Integration Results for ADC1 A, ELSD

RetTim	Width	Area	Height	Area%
7.25	0.04	2270.46	937.51	100.00

Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%
7.19	0.04	1706.34	682.79	100.00

Integration Results for DAD1 B, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%
7.19	0.04	2888.05	1140.78	98.69
7.69	0.04	19.43	7.38	0.66
7.99	0.04	10.14	3.88	0.35
8.91	0.04	8.67	3.14	0.30