
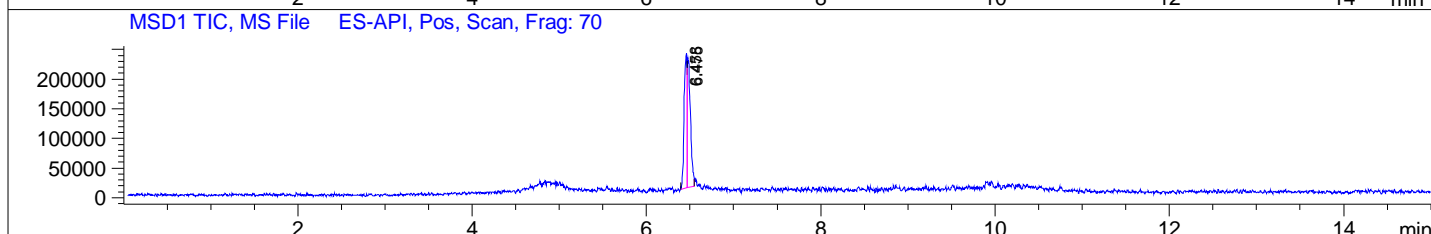
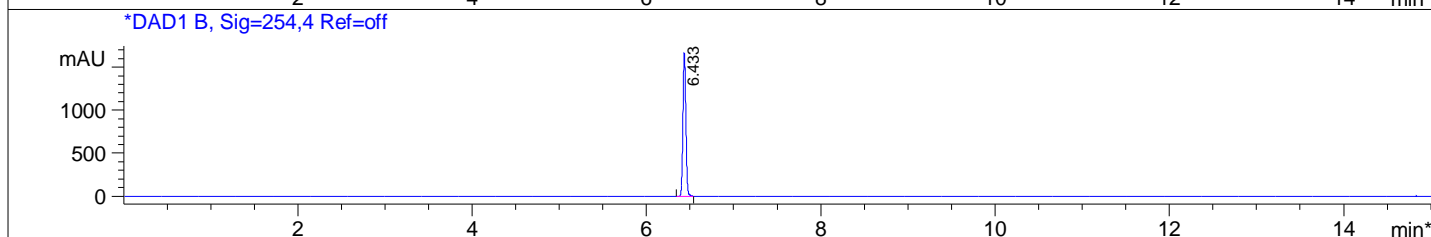
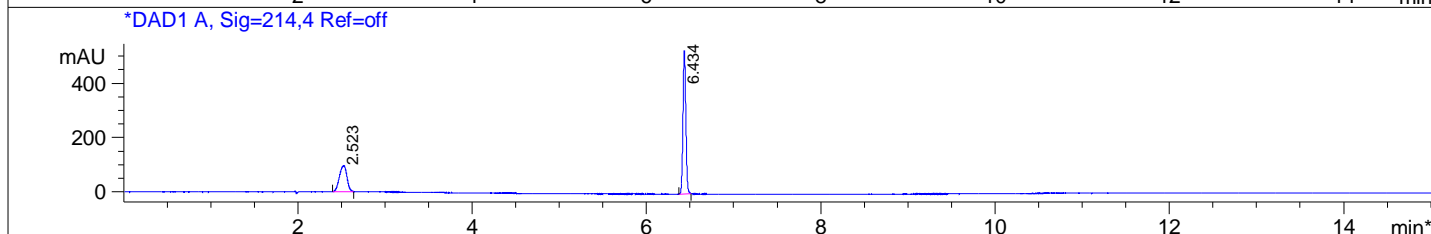


File D:\DATA\T91\MONITOR\GSK121015A-00510-HPLC  
 Injection Date : 26 Jul 12 7:06 pm +0800 Tgt Mass(EZX) :  
 Sample Name : NF-556-2 Location : P1-C-07  
 Acq. Operator : T91-Monitor Inj : 1  
 Spec. Reported : MS Integration Inj Volume : 1 ul  
 Acq. Method : C:\Chem32\1\METHODS\2-HPLC-15MIN.M  
 Analysis Method : C:\Chem32\1\METHODS\2-HPLC-15MIN.M  
 Sample Info : \*\*\* No target masses specified \*\*\*  
 Method Info : Mobile Phase : A:Water( 10mM NH4HCO3), B: Acetonitrile  
 Gradient : 5%-95% B in 8 min  
 Flow Rate : 1mL/min  
 Column : XBridge C18 ,4.6\*150mm, 3.5um  
 Oven Temperature : 40 C  
 uv214nm,mass100-1000

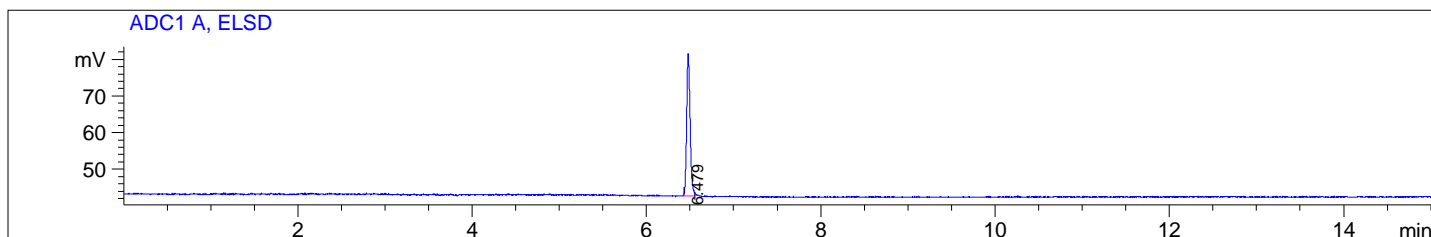

Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%
2.52	0.07	583.58	96.42	32.36
6.43	0.04	1219.81	528.05	67.64

Integration Results for DAD1 B, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%
6.43	0.03	3929.97	1669.21	100.00

Ret. Time: 6.46 <<<< POSITIVE SPECTRA >>>> Ret. Time: 6.48

