


File D:\DATA GSK429286A
 Sample Info : *** No target masses specified ***
 Method Info : Mobile Phase: A: water(10mM Ammonium hydrogen carbonate) B: ACN
 Gradient: 5%-95% B in 1.6min
 Flow Rate: 2.0ml/min
 Column: XBridge C18,4.6*50mm,3.5um
 Oven Temperature: 40 C
 MS Range: 110-800

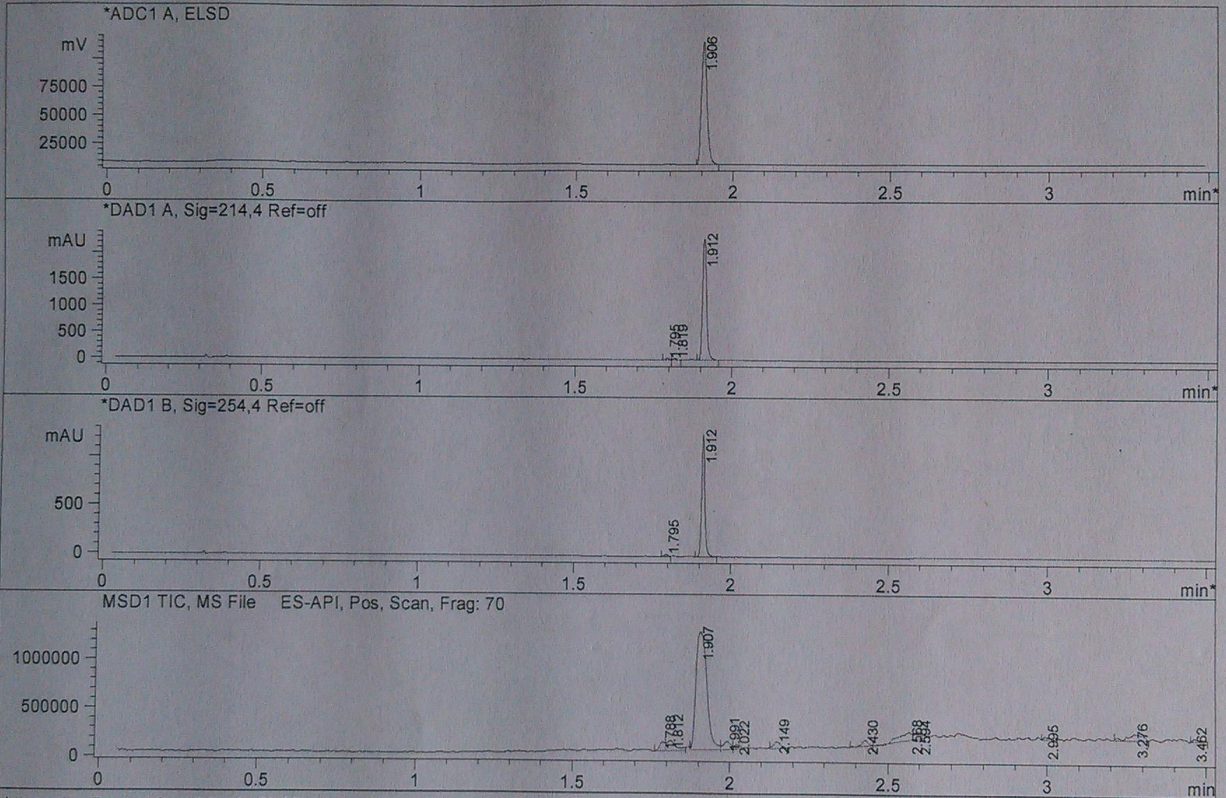

Integration Results for ADC1 A, ELSD

RetTim	Width	Area	Height	Area%
1.91	0.02	132743.27	107328.40	100.00

Integration Results for DAD1 A, Sig=214,4 Ref=off


RetTim	Width	Area	Height	Area%
1.79	0.01	29.40	37.69	1.34
1.82	0.01	22.67	31.55	1.03
1.91	0.01	2141.08	2297.72	97.63

Integration Results for DAD1 B, Sig=254,4 Ref=off


RetTim	Width	Area	Height	Area%
1.79	0.01	14.83	18.77	1.58
1.91	0.01	923.84	1255.20	98.42

Ret. Time: 1.79


<<<< POSITIVE SPECTRA >>>>

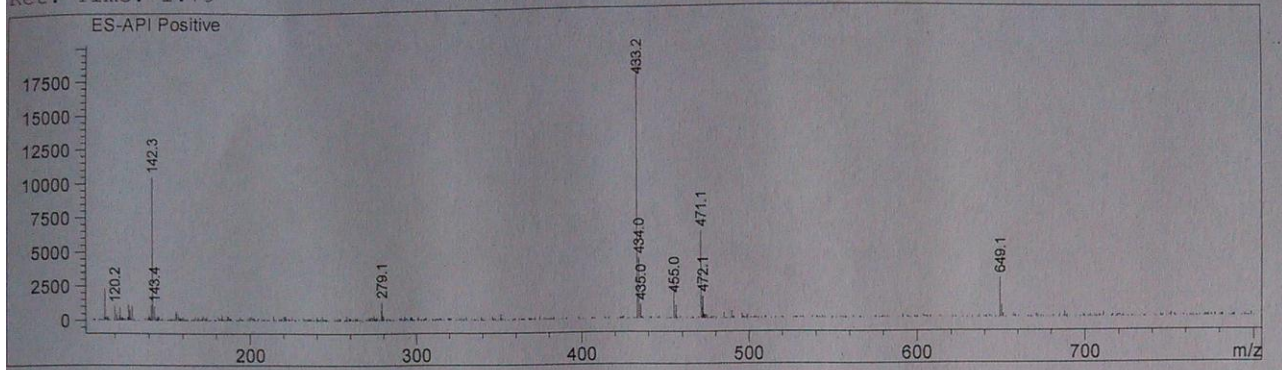

Ret. Time: 1.81

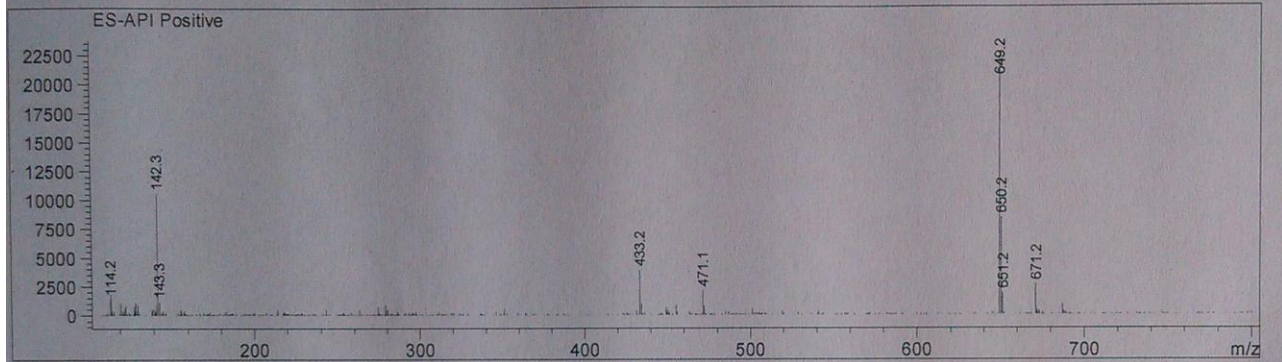

Ret. Time: 1.91

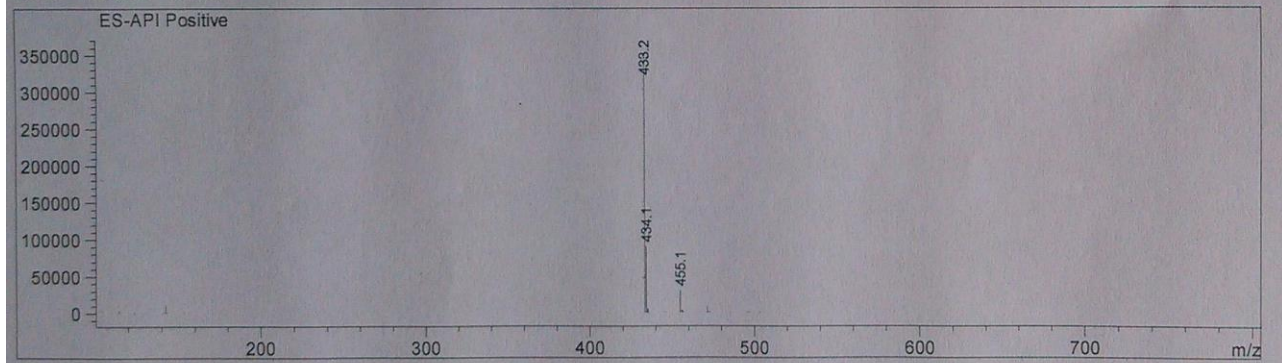

Ret. Time: 1.99

