
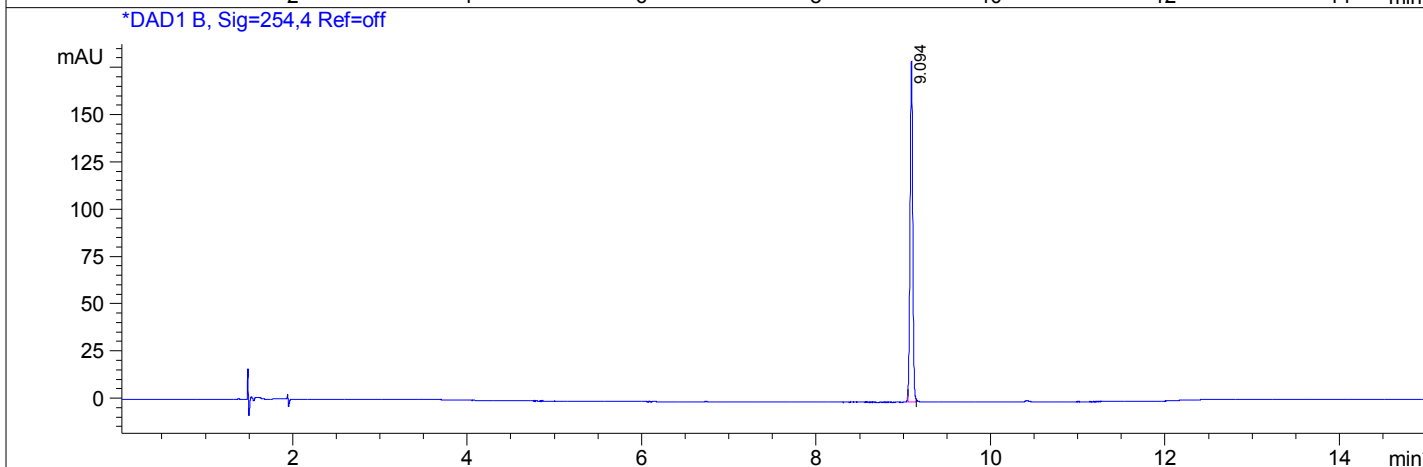


```

File D:\DAT\MONITOR\1                               Tgt Mass (EZX):\
Injection Date   : 10-Mar-16, 17:43:08             Seq. Line   : 0
Sample Name     : 1                               Location    : P1
Acq. Operator  : Monitor                          Inj         : 0
Spec. Reported  : MS Integration                   Inj Volume  : 6 ul
Acq. Method    : D:\METHODS\2-HPLC-15MIN.M
Analysis Method : D:\METHODS\2-HPLC-15MIN.M
Sample Info    : Easy-Access Method: '2-HPLC-15MIN'
Method Info    : Mobile Phase:  A: water(10mM Ammonium hydrogen carbonate)  B: ACN
                  Gradient: 0min 5%B,3min 5%B,10min 95%B,15min 95% B
                  Flow Rate: 1.2ml/min
                  Column: XBridge C18,4.6*150mm,3.5um
                  Oven Temperature: 45 C
                  MASS Range:110-800
    
```

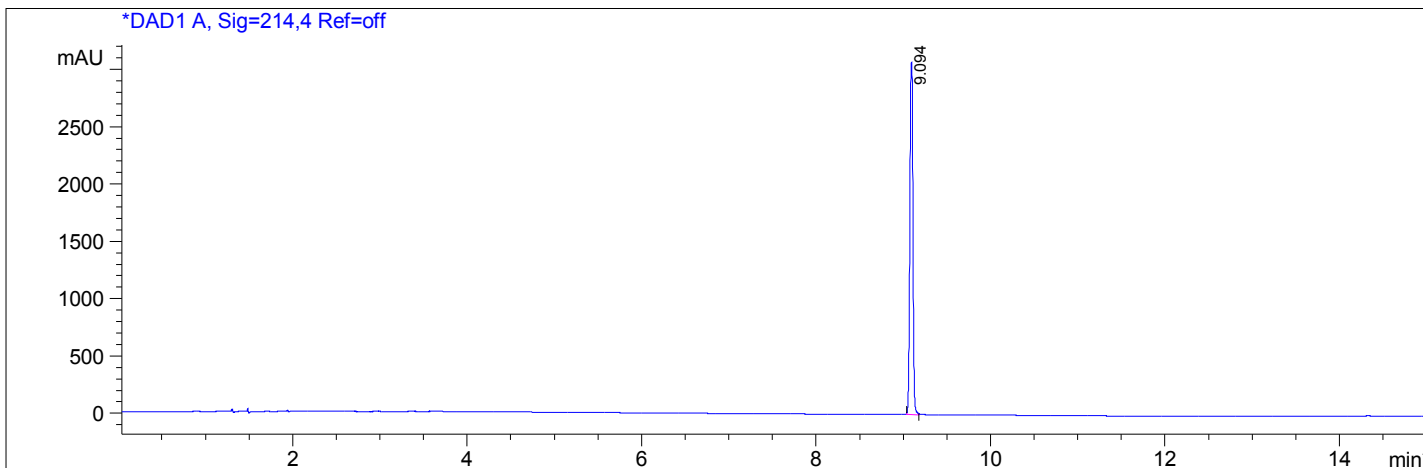

Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%
9.09	0.04	7527.64	3069.10	100.00

Integration Results for DAD1 B, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%
9.09	0.03	381.42	180.04	100.00