

File D:\DATA\

Acq. Method : C:\Chem32\1\METHODS\2-POS-CN-8MIN.M

Analysis Method : C:\Chem32\1\METHODS\2-POS-CN-8MIN.M

Sample Info : \*\*\* No target masses specified \*\*\*

Method Info : Mobile Phase: A: water(0.01%TFA) B: ACN(0.01%TFA)

Gradient: 5%-95% B in 6.0min


Flow Rate: 1.5ml/min

Column: Waters CNRP 4.6x 150 mm, 5um


Column Temperature: 35 C

MASS Range:80-1000


ADC1 A, ELSD

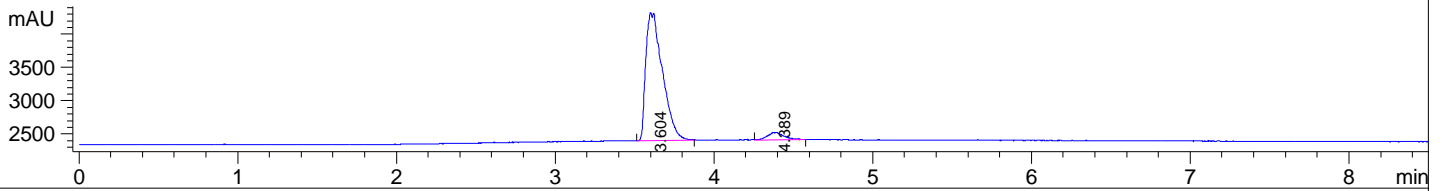


DAD1 A, Sig=214,4 Ref=off

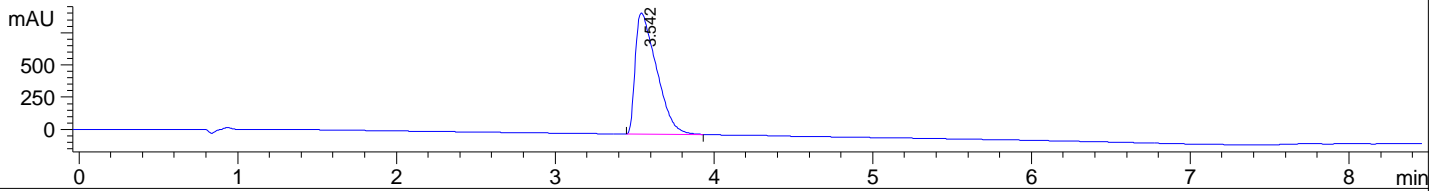

DAD1 B, Sig=254,4 Ref=off

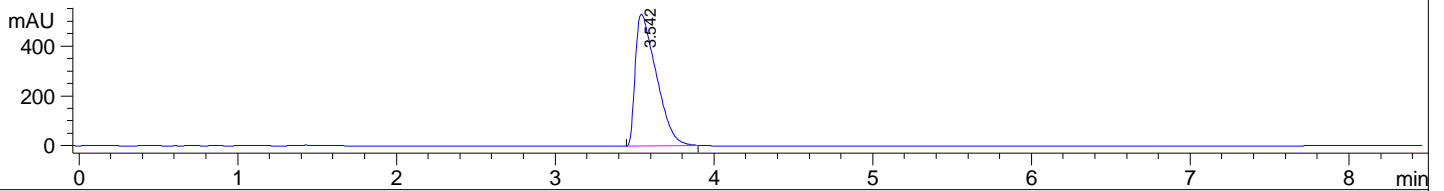

MSD1 TIC, MS File ES-API, Scan, Frag: 80

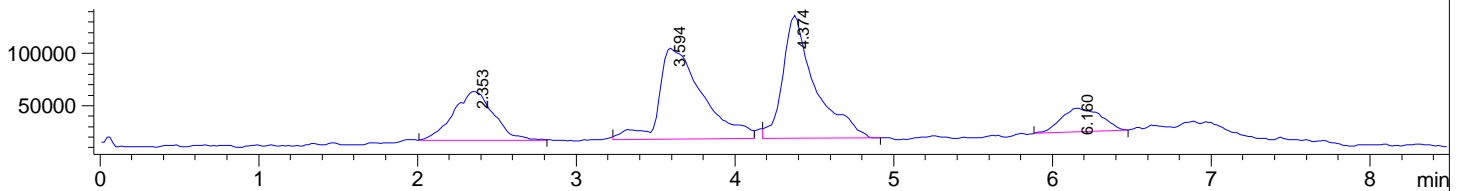

Integration Results for ADC1 A, ELSD

RetTim	Width	Area	Height	Area%
3.60	0.10	14040.33	1909.28	94.48
4.39	0.10	820.51	110.92	5.52


Integration Results for DAD1 A, Sig=214,4 Ref=off

RetTim	Width	Area	Height	Area%
3.54	0.15	8729.54	941.06	100.00


Integration Results for DAD1 B, Sig=254,4 Ref=off

RetTim	Width	Area	Height	Area%
3.54	0.15	4873.41	530.74	100.00


Ret. Time: 2.35 <<<< POSITIVE SPECTRA >>>>

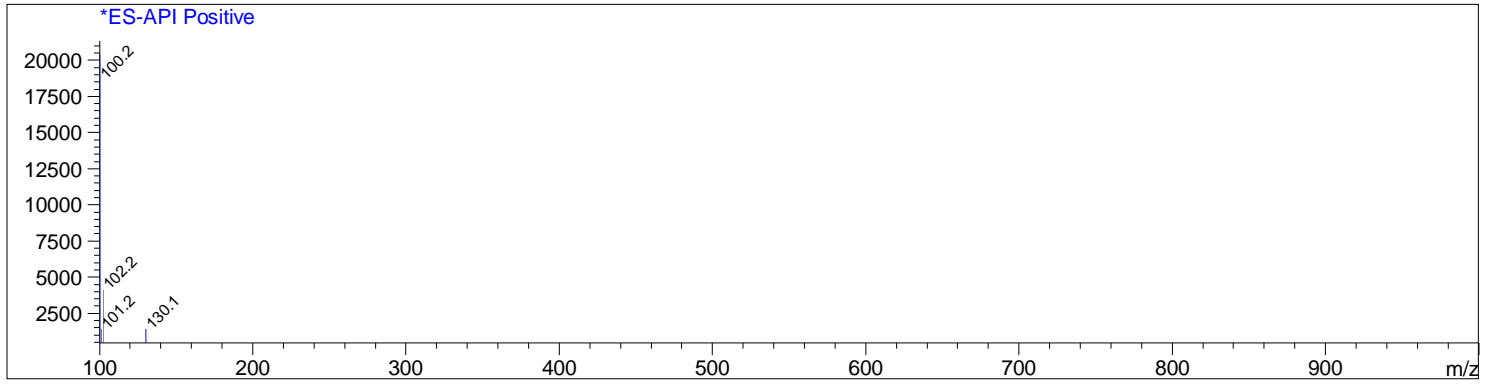

Ret. Time: 3.59

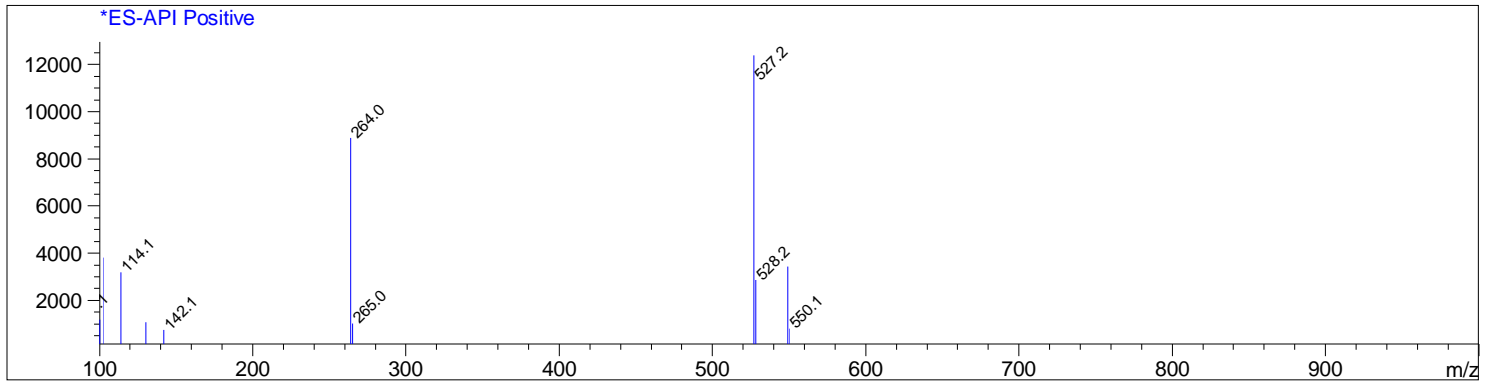

Ret. Time: 4.37

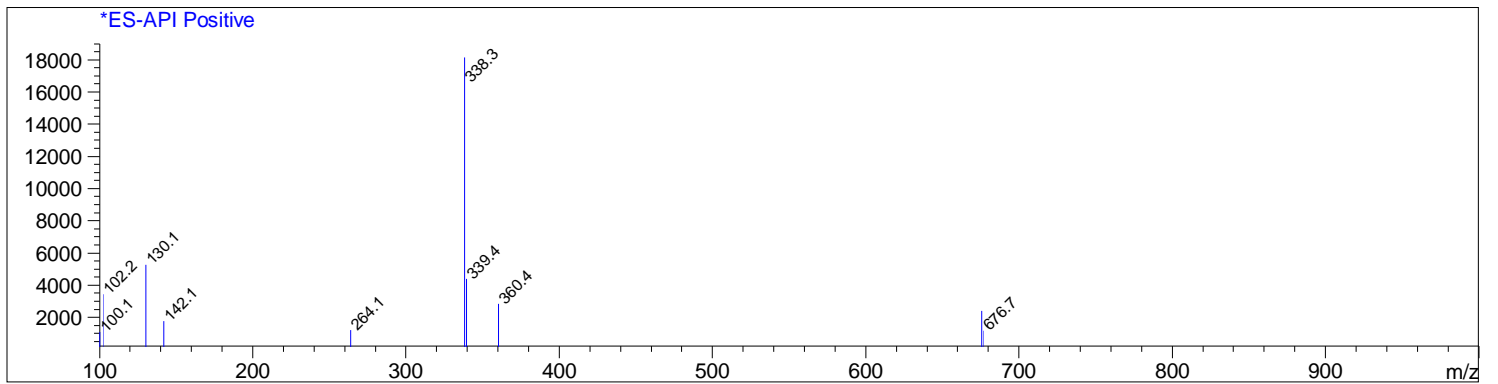

Ret. Time: 6.16

